

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021893.D
 Acq On : 19 Aug 2021 16:47
 Operator : SY/MD
 Sample : M3448-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG5

Quant Time: Aug 20 02:18:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 20 02:14:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	480454	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	435988	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	208213	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	131931	35.125	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.260%		
7) Chloroethane-d5	1.558	69	106036	37.410	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	74.820%		
11) 1,1-Dichloroethene-d2	2.105	63	165862	27.742	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.480%#		
21) 2-Butanone-d5	3.873	46	213493	91.392	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.390%		
24) Chloroform-d	4.352	84	253687	38.984	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.960%		
26) 1,2-Dichloroethane-d4	5.034	65	156314	41.760	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.520%		
32) Benzene-d6	5.050	84	543562	43.355	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.720%		
36) 1,2-Dichloropropane-d6	6.072	67	171168	43.841	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.680%		
41) Toluene-d8	7.317	98	496109	42.812	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.620%		
43) trans-1,3-Dichloroprop...	7.625	79	74977	39.020	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.040%		
47) 2-Hexanone-d5	8.088	63	120062	93.826	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.830%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	221107	45.700	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.400%		
66) 1,2-Dichlorobenzene-d4	11.625	152	194679	45.179	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.360%		
Target Compounds					Qvalue	
13) Acetone	2.159	43	5690	2.960	ug/L #	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021893.D
Acq On : 19 Aug 2021 16:47
Operator : SY/MD
Sample : M3448-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG5


Quant Time: Aug 20 02:18:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 20 02:14:47 2021
Response via : Initial Calibration

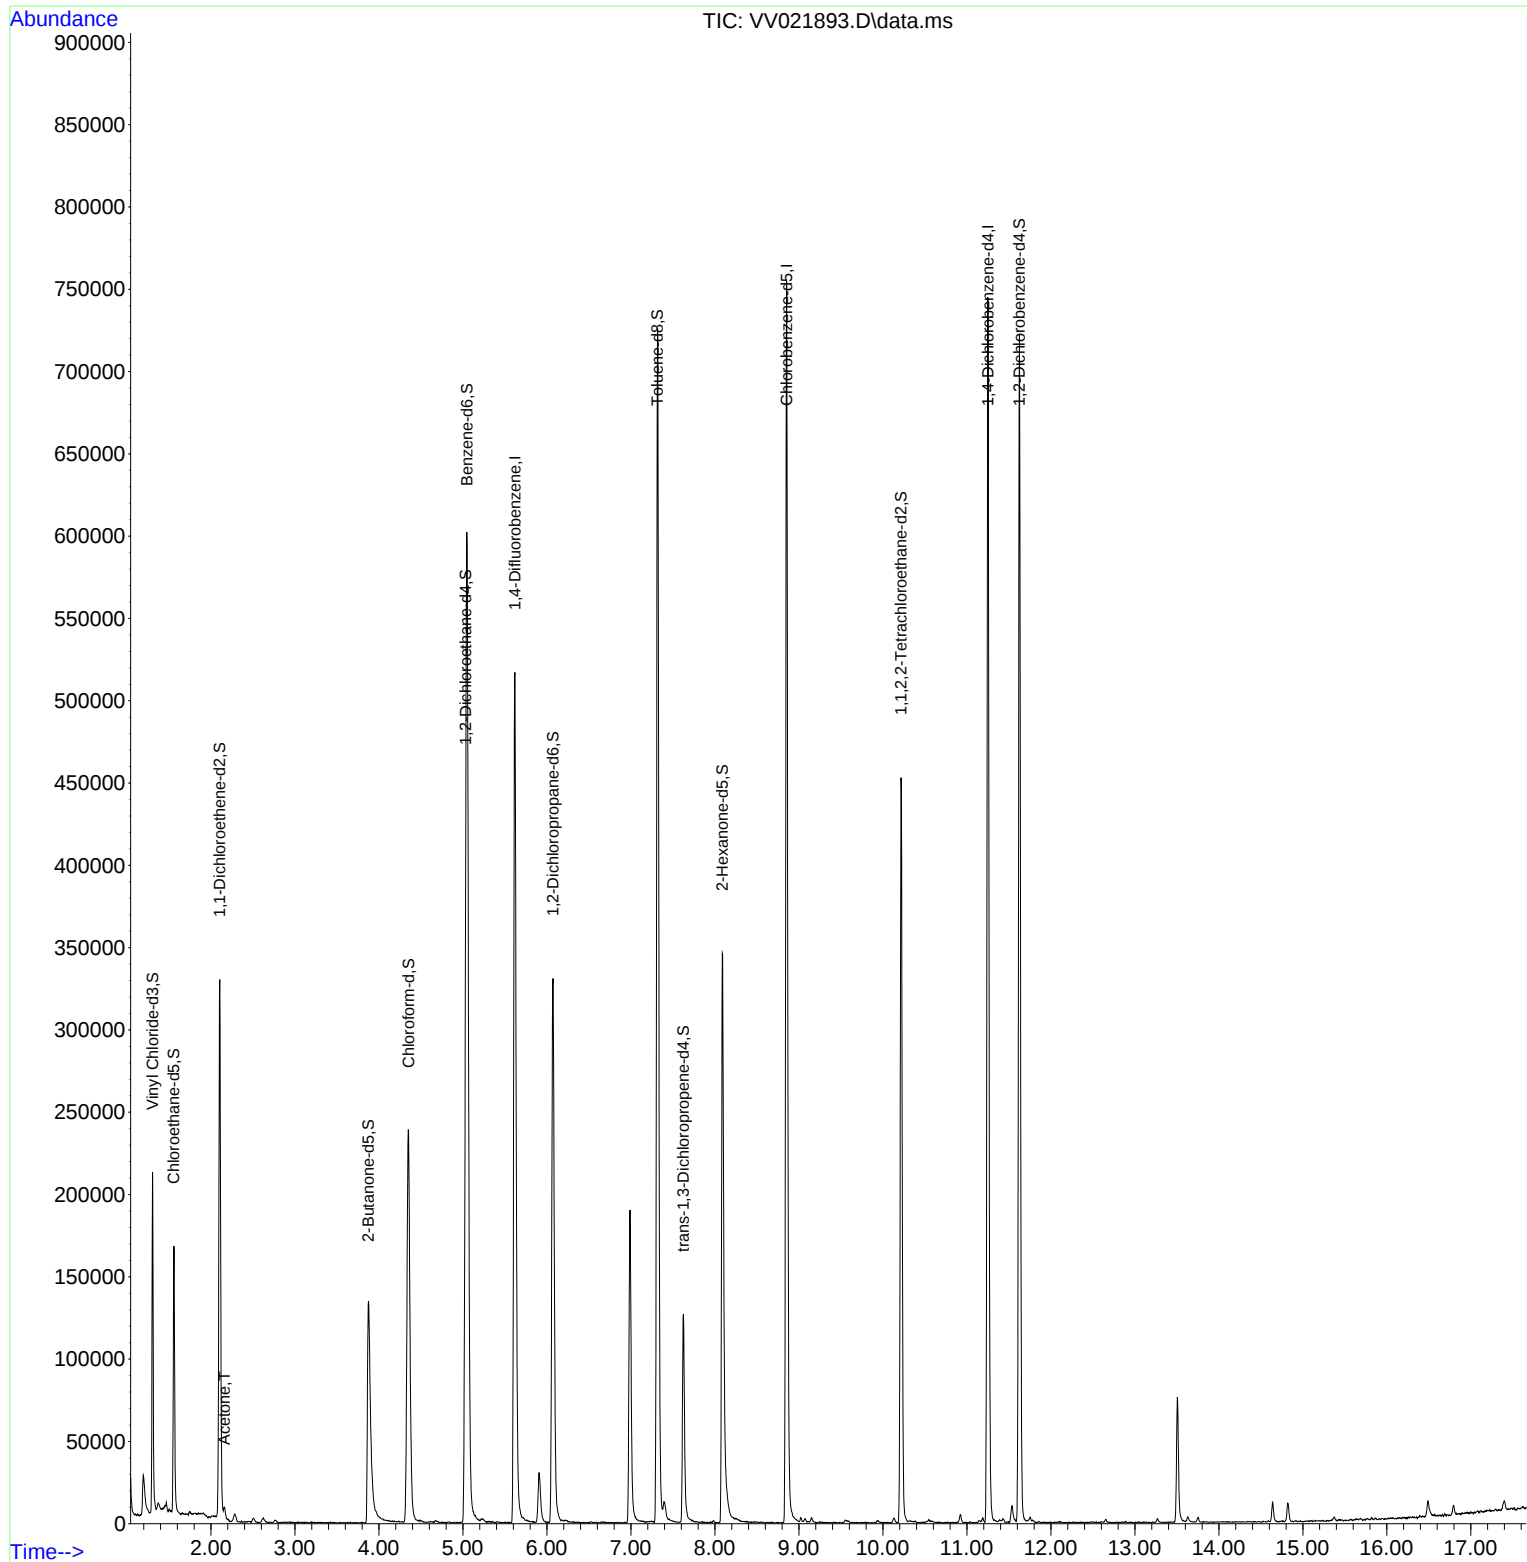

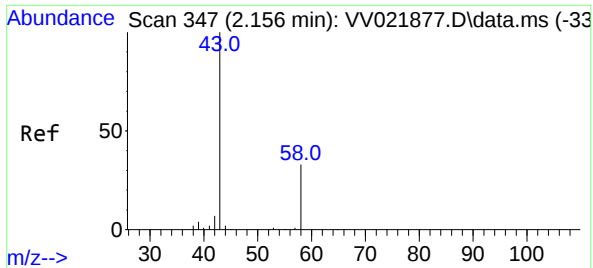

#13
Acetone
Concen: 2.960 ug/L
RT: 2.159 min Scan# 348
Delta R.T. 0.003 min
Lab File: VV021893.D
Acq: 19 Aug 2021 16:47

Instrument :
MSVOA_V
ClientSampleId :
DBKG5

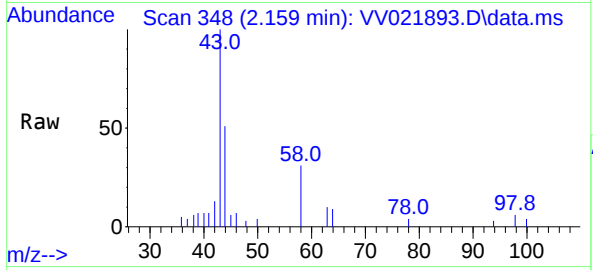

Tgt Ion: 43 Resp: 5690
Ion Ratio Lower Upper
43 100
58 33.3 0.0 0.0#

