

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021895.D
 Acq On : 19 Aug 2021 17:36
 Operator : SY/MD
 Sample : M3448-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M

Title : VOC Analysis

Signal : TIC: VV021895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	223636	212747	14.21%	1.830%
2	1.561	155	162	176	rVB	165193	190749	12.74%	1.640%
3	2.105	321	331	347	rBV	331539	482029	32.20%	4.145%
4	2.336	401	403	406	rBV2	712	454	0.03%	0.004%
5	2.384	415	418	420	rBV2	514	356	0.02%	0.003%
6	2.744	525	530	531	rBV3	386	298	0.02%	0.003%
7	2.825	553	555	558	rBV	334	179	0.01%	0.002%
8	2.941	589	591	595	rVB2	367	192	0.01%	0.002%
9	2.992	603	607	609	rBV3	517	283	0.02%	0.002%
10	3.053	623	626	629	rBV3	585	419	0.03%	0.004%
11	3.163	655	660	665	rBV	235	228	0.02%	0.002%
12	3.291	698	700	704	rBV2	378	209	0.01%	0.002%
13	3.407	733	736	740	rBV2	299	251	0.02%	0.002%
14	3.471	753	756	758	rBV3	340	238	0.02%	0.002%
15	3.622	800	803	805	rBV2	270	165	0.01%	0.001%
16	3.735	834	838	841	rVB	435	223	0.01%	0.002%
17	3.818	861	864	868	rBV2	298	196	0.01%	0.002%
18	3.841	868	871	872	rBV	317	175	0.01%	0.002%
19	3.876	872	882	914	rBV	120438	323674	21.62%	2.783%
20	4.349	1014	1029	1066	rVB	233679	579057	38.68%	4.980%
21	4.587	1101	1103	1109	rVB3	423	356	0.02%	0.003%
22	4.696	1136	1137	1141	rVB	781	239	0.02%	0.002%
23	4.770	1156	1160	1162	rBV3	450	260	0.02%	0.002%
24	4.802	1167	1170	1176	rVB2	411	429	0.03%	0.004%
25	4.838	1180	1181	1187	rVB	294	160	0.01%	0.001%
26	4.899	1197	1200	1203	rVB2	367	222	0.01%	0.002%
27	5.047	1227	1246	1276	rBV2	586991	1497058	100.00%	12.874%
28	5.426	1360	1364	1369	rVB4	731	654	0.04%	0.006%
29	5.619	1411	1424	1460	rBV	502030	1017251	67.95%	8.748%
30	5.908	1505	1514	1532	rVB	18550	37994	2.54%	0.327%
31	6.072	1551	1565	1586	rBV	327508	662871	44.28%	5.700%
32	6.268	1621	1626	1632	rVB4	803	930	0.06%	0.008%
33	6.297	1632	1635	1640	rVV3	640	394	0.03%	0.003%
34	6.320	1640	1642	1645	rVB2	566	285	0.02%	0.002%
35	6.342	1645	1649	1651	rBV3	414	260	0.02%	0.002%
36	6.423	1672	1674	1677	rBV2	221	157	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021895.D
 Acq On : 19 Aug 2021 17:36
 Operator : SY/MD
 Sample : M3448-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

37	6.465	1684	1687	1689	rBV2	517	278	0.02%	0.002%
38	6.645	1738	1743	1745	rBV4	528	491	0.03%	0.004%
39	6.751	1773	1776	1780	rVB2	385	339	0.02%	0.003%
40	6.805	1789	1793	1794	rVV2	250	196	0.01%	0.002%

41	6.818	1794	1797	1802	rVB3	392	306	0.02%	0.003%
42	6.905	1822	1824	1827	rBV	279	165	0.01%	0.001%
43	6.989	1838	1850	1885	rBV	183442	336037	22.45%	2.890%
44	7.185	1907	1911	1913	rBV3	517	441	0.03%	0.004%
45	7.246	1928	1930	1934	rVB3	945	573	0.04%	0.005%

46	7.317	1939	1952	1971	rBV	707030	1229849	82.15%	10.576%
47	7.625	2038	2048	2073	rBV	117300	208453	13.92%	1.793%
48	7.873	2122	2125	2128	rBV3	508	318	0.02%	0.003%
49	7.944	2140	2147	2154	rBV5	2998	4782	0.32%	0.041%
50	7.995	2161	2163	2166	rVB2	550	260	0.02%	0.002%

51	8.088	2181	2192	2223	rBV	335235	620096	41.42%	5.333%
52	8.365	2276	2278	2285	rVB3	649	614	0.04%	0.005%
53	8.397	2285	2288	2290	rBV3	402	262	0.02%	0.002%
54	8.423	2294	2296	2298	rBV2	359	160	0.01%	0.001%
55	8.484	2311	2315	2319	rBV4	647	581	0.04%	0.005%

56	8.593	2346	2349	2352	rVB	419	270	0.02%	0.002%
57	8.625	2352	2359	2363	rBV5	626	794	0.05%	0.007%
58	8.744	2391	2396	2399	rBV3	371	384	0.03%	0.003%
59	8.805	2412	2415	2419	rBV2	408	283	0.02%	0.002%
60	8.854	2419	2430	2458	rBV	734762	1192628	79.66%	10.256%

61	9.233	2546	2548	2550	rBV3	361	165	0.01%	0.001%
62	9.265	2556	2558	2561	rVB3	354	168	0.01%	0.001%
63	9.323	2573	2576	2578	rBV	302	187	0.01%	0.002%
64	9.461	2616	2619	2624	rVB	287	176	0.01%	0.002%
65	9.558	2640	2649	2655	rBV6	949	1300	0.09%	0.011%

66	9.812	2725	2728	2730	rVB	349	160	0.01%	0.001%
67	9.834	2730	2735	2736	rBV2	276	191	0.01%	0.002%
68	9.844	2736	2738	2743	rVB2	228	157	0.01%	0.001%
69	9.937	2763	2767	2770	rBV3	566	516	0.03%	0.004%
70	10.130	2819	2827	2838	rBV4	3062	4774	0.32%	0.041%

71	10.217	2843	2854	2875	rVV	449283	715234	47.78%	6.151%
72	10.384	2897	2906	2917	rVB	4855	7277	0.49%	0.063%
73	10.464	2928	2931	2933	rBV2	547	366	0.02%	0.003%
74	10.538	2952	2954	2960	rVB3	587	467	0.03%	0.004%
75	10.747	3017	3019	3026	rVB3	298	215	0.01%	0.002%

76	10.780	3026	3029	3032	rVB3	362	185	0.01%	0.002%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021895.D
 Acq On : 19 Aug 2021 17:36
 Operator : SY/MD
 Sample : M3448-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

77	10.805	3032	3037	3040	rBV2	440	398	0.03%	0.003%
78	10.924	3065	3074	3083	rVV5	3510	5148	0.34%	0.044%
79	10.989	3089	3094	3098	rBV2	238	297	0.02%	0.003%
80	11.034	3105	3108	3111	rBV2	581	444	0.03%	0.004%
81	11.149	3138	3144	3152	rBV5	1526	2143	0.14%	0.018%
82	11.252	3164	3176	3207	rBV	705190	1124657	75.12%	9.672%
83	11.468	3240	3243	3247	rBV2	340	280	0.02%	0.002%
84	11.535	3256	3264	3274	rBV4	3475	6260	0.42%	0.054%
85	11.625	3280	3292	3318	rBV	681045	1083323	72.36%	9.316%
86	11.934	3386	3388	3391	rBV	470	237	0.02%	0.002%
87	11.950	3391	3393	3400	rVB2	469	389	0.03%	0.003%
88	11.992	3400	3406	3407	rBV	374	312	0.02%	0.003%
89	12.030	3413	3418	3419	rBV3	439	342	0.02%	0.003%
90	12.423	3538	3540	3544	rBV2	281	183	0.01%	0.002%
91	12.480	3556	3558	3560	rBV	364	199	0.01%	0.002%
92	12.606	3594	3597	3599	rBV	332	212	0.01%	0.002%
93	12.651	3609	3611	3613	rBV2	371	164	0.01%	0.001%
94	12.802	3656	3658	3664	rVB2	310	178	0.01%	0.002%
95	12.886	3682	3684	3688	rBV2	384	303	0.02%	0.003%
96	13.262	3799	3801	3803	rBV2	447	226	0.02%	0.002%
97	13.509	3869	3878	3900	rVB	33408	55232	3.69%	0.475%
98	13.805	3965	3970	3972	rBV3	567	543	0.04%	0.005%
99	14.644	4223	4231	4241	rVB3	2930	4860	0.32%	0.042%
100	15.149	4386	4388	4390	rBV2	816	336	0.02%	0.003%


Sum of corrected areas: 11628406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021895.D
Acq On : 19 Aug 2021 17:36
Operator : SY/MD
Sample : M3448-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

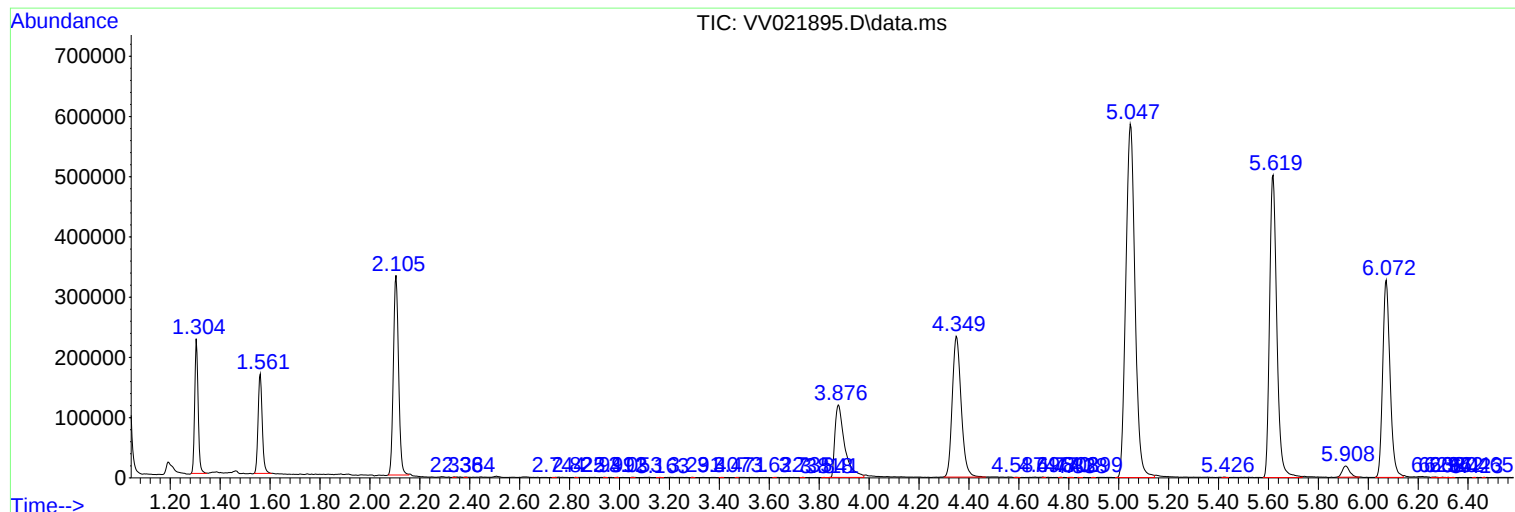

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021895.D
Acq On : 19 Aug 2021 17:36
Operator : SY/MD
Sample : M3448-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021895.D
Acq On : 19 Aug 2021 17:36
Operator : SY/MD
Sample : M3448-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
