

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021897.D
 Acq On : 19 Aug 2021 18:24
 Operator : SY/MD
 Sample : M3448-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

Signal : TIC: VV021897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rBV	204409	203347	13.59%	1.716%
2	1.561	155	162	179	rVB	161614	190814	12.76%	1.610%
3	2.105	322	331	344	rVB	322632	464003	31.02%	3.915%
4	2.484	446	449	450	rBV2	789	450	0.03%	0.004%
5	2.507	451	456	463	rVB5	1494	2174	0.15%	0.018%
6	2.610	486	488	489	rBV	451	204	0.01%	0.002%
7	2.770	525	538	550	rBV2	14971	32194	2.15%	0.272%
8	2.851	561	563	566	rVB3	423	201	0.01%	0.002%
9	2.954	593	595	600	rVB2	313	221	0.01%	0.002%
10	3.021	613	616	619	rBV	501	298	0.02%	0.003%
11	3.044	621	623	628	rVB3	376	255	0.02%	0.002%
12	3.130	647	650	652	rBV2	315	219	0.01%	0.002%
13	3.182	664	666	668	rBV	295	177	0.01%	0.001%
14	3.275	693	695	697	rBV	352	184	0.01%	0.002%
15	3.359	719	721	726	rBV2	315	206	0.01%	0.002%
16	3.581	786	790	794	rBV2	326	298	0.02%	0.003%
17	3.873	871	881	919	rBV	124737	329226	22.01%	2.778%
18	4.349	1015	1029	1061	rVB	233419	576138	38.52%	4.861%
19	4.671	1127	1129	1131	rBV	487	269	0.02%	0.002%
20	4.722	1141	1145	1146	rBV	478	332	0.02%	0.003%
21	4.748	1150	1153	1157	rBV	498	309	0.02%	0.003%
22	4.777	1157	1162	1165	rBV3	329	292	0.02%	0.002%
23	4.857	1185	1187	1192	rVB2	504	335	0.02%	0.003%
24	4.960	1215	1219	1223	rBV	356	241	0.02%	0.002%
25	5.047	1229	1246	1271	rBV2	585315	1495849	100.00%	12.620%
26	5.433	1364	1366	1370	rBV2	406	238	0.02%	0.002%
27	5.535	1395	1398	1400	rVB3	347	194	0.01%	0.002%
28	5.564	1400	1407	1410	rBV4	552	536	0.04%	0.005%
29	5.616	1410	1423	1455	rBV	502489	1021068	68.26%	8.615%
30	5.908	1504	1514	1533	rVB3	11421	25441	1.70%	0.215%
31	6.005	1541	1544	1547	rVB3	728	412	0.03%	0.003%
32	6.072	1547	1565	1597	rBV	330707	675175	45.14%	5.696%
33	6.301	1634	1636	1640	rBV2	414	312	0.02%	0.003%
34	6.349	1648	1651	1654	rBV3	598	354	0.02%	0.003%
35	6.404	1664	1668	1671	rBV2	246	207	0.01%	0.002%
36	6.432	1676	1677	1680	rVB2	415	173	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021897.D
 Acq On : 19 Aug 2021 18:24
 Operator : SY/MD
 Sample : M3448-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

37	6.484	1691	1693	1698	rVB2	341	231	0.02%	0.002%
38	6.513	1698	1702	1704	rBV	362	220	0.01%	0.002%
39	6.757	1775	1778	1782	rBV2	455	368	0.02%	0.003%
40	6.828	1797	1800	1803	rVB	284	204	0.01%	0.002%
41	6.860	1805	1810	1812	rBV2	357	229	0.02%	0.002%
42	6.931	1829	1832	1836	rBV3	335	314	0.02%	0.003%
43	6.989	1836	1850	1875	rBV	182362	333394	22.29%	2.813%
44	7.317	1940	1952	1970	rBV	707535	1231703	82.34%	10.392%
45	7.625	2037	2048	2065	rBV	119980	207099	13.84%	1.747%
46	7.870	2120	2124	2128	rBV3	319	337	0.02%	0.003%
47	7.944	2135	2147	2155	rBV5	3619	7363	0.49%	0.062%
48	8.027	2170	2173	2176	rBV2	203	174	0.01%	0.001%
49	8.088	2182	2192	2231	rBV	340117	621832	41.57%	5.246%
50	8.339	2268	2270	2273	rVB2	763	341	0.02%	0.003%
51	8.429	2294	2298	2299	rBV	453	326	0.02%	0.003%
52	8.561	2337	2339	2344	rVB2	449	367	0.02%	0.003%
53	8.677	2372	2375	2377	rBV2	337	189	0.01%	0.002%
54	8.738	2391	2394	2398	rVB3	364	259	0.02%	0.002%
55	8.773	2398	2405	2408	rBV2	385	349	0.02%	0.003%
56	8.854	2418	2430	2461	rBV	752055	1214284	81.18%	10.245%
57	9.069	2493	2497	2500	rBV4	393	305	0.02%	0.003%
58	9.146	2517	2521	2524	rBV5	1546	1426	0.10%	0.012%
59	9.214	2539	2542	2546	rBV	287	203	0.01%	0.002%
60	9.323	2573	2576	2579	rBV	400	237	0.02%	0.002%
61	9.471	2620	2622	2624	rBV	359	190	0.01%	0.002%
62	9.555	2641	2648	2651	rBV5	1028	1339	0.09%	0.011%
63	9.931	2762	2765	2769	rVV2	378	352	0.02%	0.003%
64	10.069	2805	2808	2810	rBV	368	182	0.01%	0.002%
65	10.127	2818	2826	2838	rVB2	2924	4234	0.28%	0.036%
66	10.217	2838	2854	2878	rBV	469360	740127	49.48%	6.244%
67	10.458	2925	2929	2930	rBV	302	215	0.01%	0.002%
68	10.747	3011	3019	3023	rBV2	1921	2395	0.16%	0.020%
69	10.786	3027	3031	3033	rVB2	259	170	0.01%	0.001%
70	10.805	3033	3037	3040	rVB3	340	236	0.02%	0.002%
71	10.821	3040	3042	3044	rBV2	291	171	0.01%	0.001%
72	10.860	3052	3054	3056	rVB2	419	184	0.01%	0.002%
73	10.924	3067	3074	3087	rVB6	3232	4726	0.32%	0.040%
74	10.995	3091	3096	3099	rBV2	447	345	0.02%	0.003%
75	11.027	3103	3106	3107	rBV	674	343	0.02%	0.003%
76	11.149	3136	3144	3150	rVB7	1226	1813	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021897.D
 Acq On : 19 Aug 2021 18:24
 Operator : SY/MD
 Sample : M3448-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis

77	11.188	3150	3156	3161	rBV5	1000	908	0.06%	0.008%
78	11.249	3164	3175	3202	rBV	742059	1159068	77.49%	9.779%
79	11.419	3226	3228	3229	rBV2	1280	566	0.04%	0.005%
80	11.532	3252	3263	3278	rBV	40308	64638	4.32%	0.545%
81	11.625	3280	3292	3317	rVV	707123	1110520	74.24%	9.369%
82	11.950	3391	3393	3400	rVB2	370	221	0.01%	0.002%
83	12.056	3420	3426	3435	rVB4	1920	2511	0.17%	0.021%
84	12.117	3435	3445	3460	rBV2	10748	16973	1.13%	0.143%
85	12.188	3463	3467	3470	rBV3	369	334	0.02%	0.003%
86	12.252	3478	3487	3488	rBV2	1076	1138	0.08%	0.010%
87	12.365	3515	3522	3532	rVV6	2511	3308	0.22%	0.028%
88	12.477	3547	3557	3567	rBV8	3513	8283	0.55%	0.070%
89	12.728	3628	3635	3646	rBV3	5699	8502	0.57%	0.072%
90	12.889	3676	3685	3697	rBV	9857	13608	0.91%	0.115%
91	12.956	3699	3706	3717	rVB6	1867	3069	0.21%	0.026%
92	13.056	3729	3737	3748	rVB9	3917	6914	0.46%	0.058%
93	13.124	3756	3758	3762	rVB2	327	189	0.01%	0.002%
94	13.159	3766	3769	3772	rVB2	457	277	0.02%	0.002%
95	13.204	3781	3783	3784	rBV	799	388	0.03%	0.003%
96	13.313	3814	3817	3819	rBV2	672	522	0.03%	0.004%
97	13.419	3848	3850	3857	rBV2	364	315	0.02%	0.003%
98	13.509	3868	3878	3899	rVB2	25372	47326	3.16%	0.399%
99	13.860	3984	3987	3989	rBV	356	196	0.01%	0.002%
100	14.095	4055	4060	4067	rBV5	1419	1731	0.12%	0.015%




Sum of corrected areas: 11852627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021897.D
Acq On : 19 Aug 2021 18:24
Operator : SY/MD
Sample : M3448-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
DBKG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

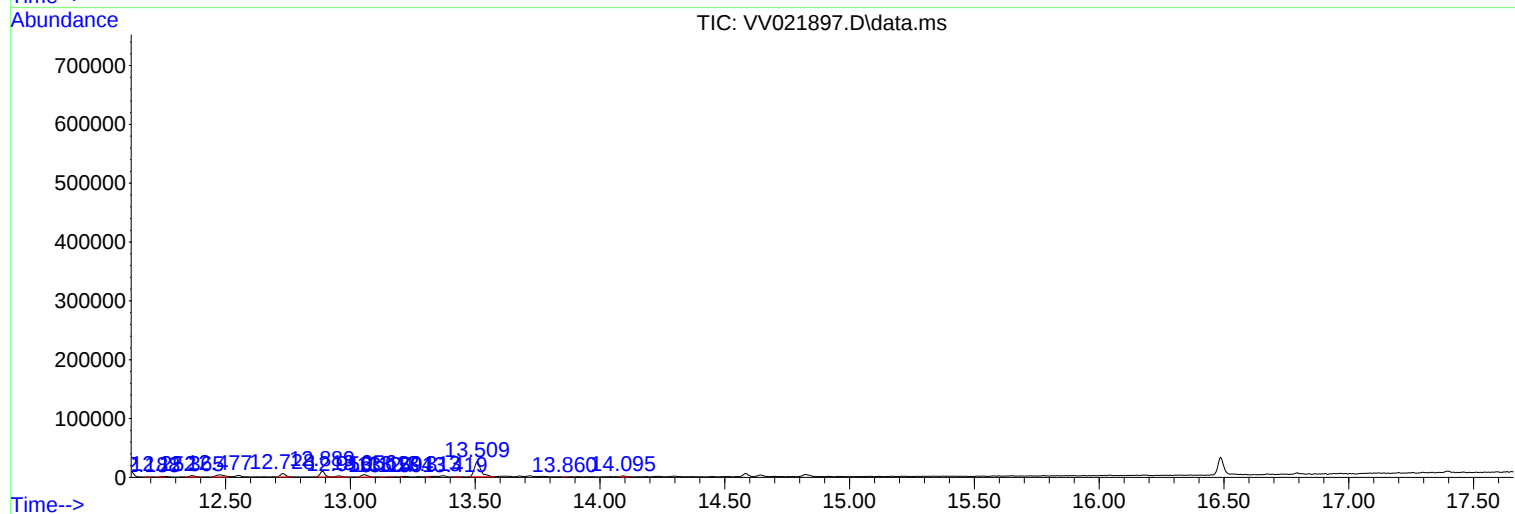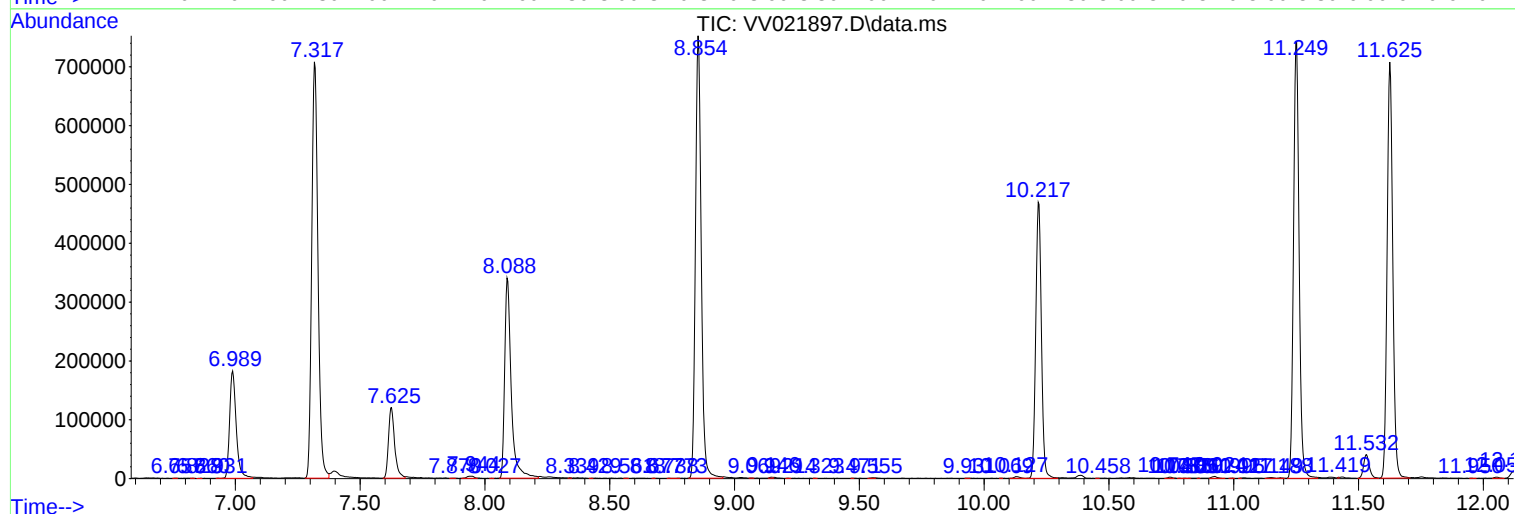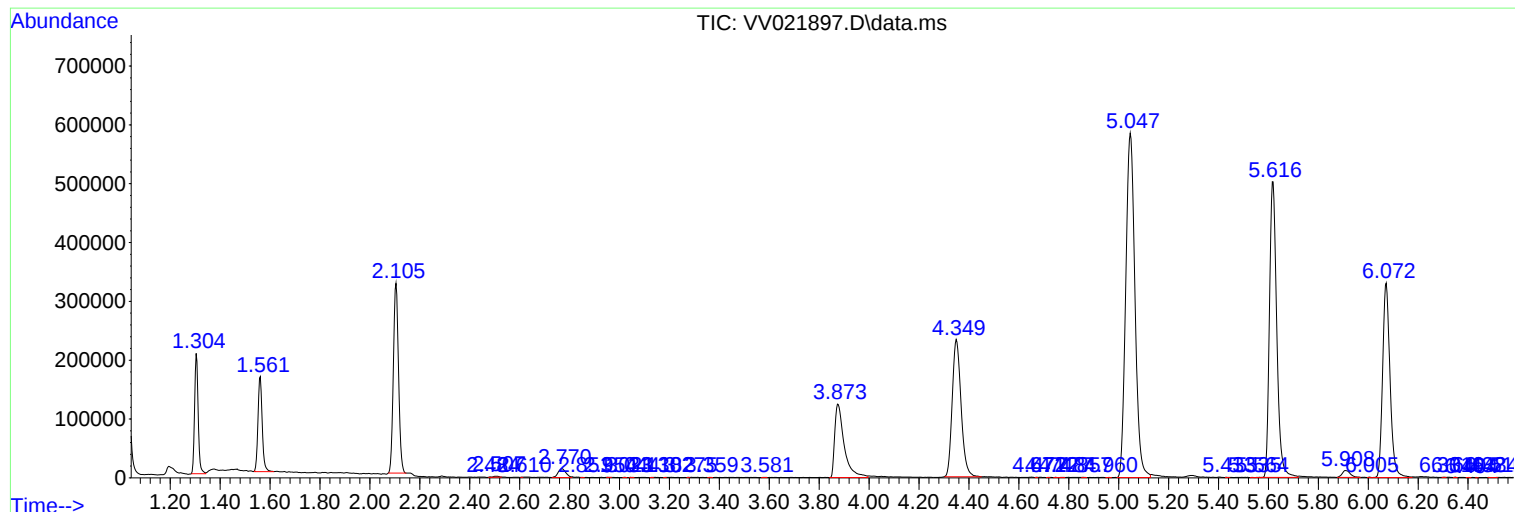

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021897.D
Acq On : 19 Aug 2021 18:24
Operator : SY/MD
Sample : M3448-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Indane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.532	2.79 ug/L	64638	1,4-Dichlorobenzene-d4	11.252

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	95
2			Benzene, cyclopropyl-	118	C9H10	000873-49-4	81
3			Benzene, 1-propenyl-	118	C9H10	000637-50-3	74
4			Benzene, 2-propenyl-	118	C9H10	000300-57-2	74
5			1,3-Methanopentalene, 1,2,3,5-te...	118	C9H10	128600-88-4	72

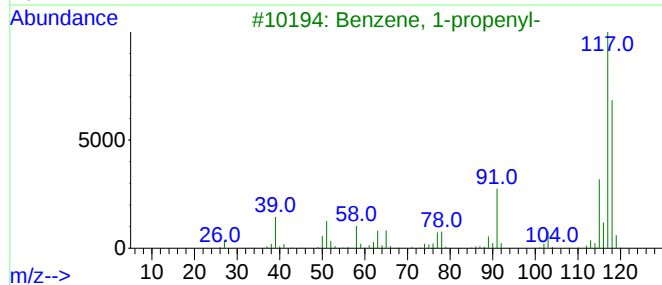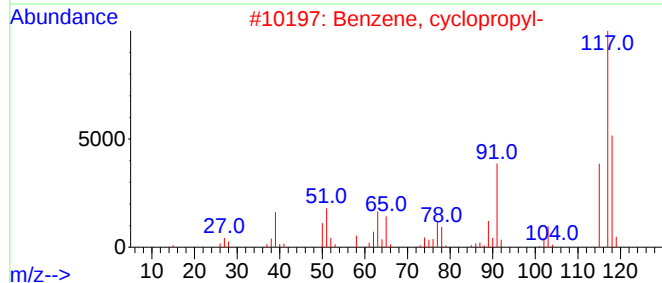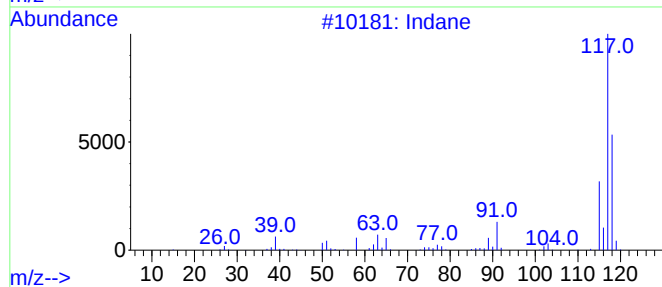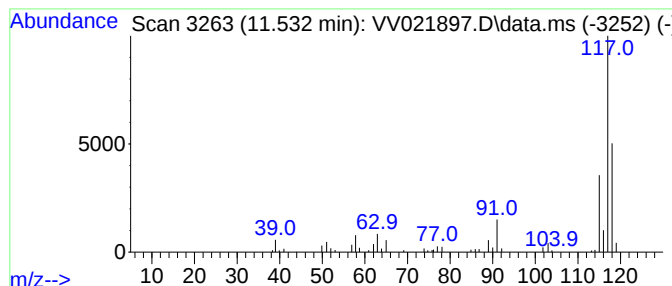

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
Data File : VV021897.D
Acq On : 19 Aug 2021 18:24
Operator : SY/MD
Sample : M3448-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	11.532	2.8	ug/L	64638	3	11.252	1159070	50.0