
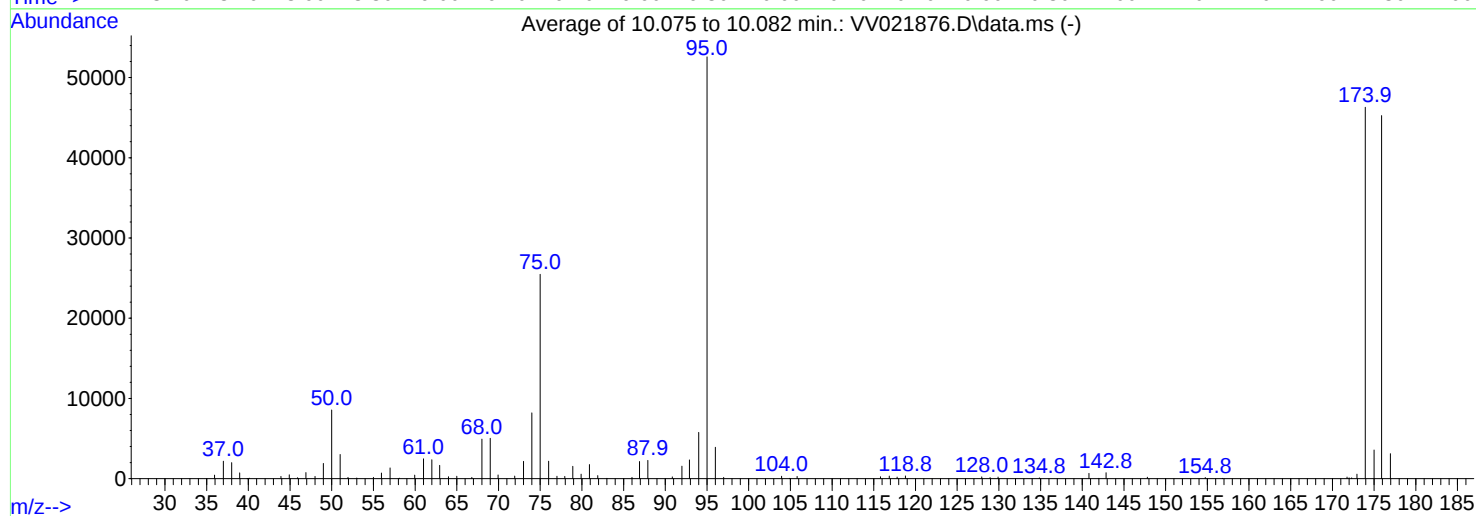


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081921\
 Data File : VV021876.D
 Acq On : 19 Aug 2021 08:56
 Operator : SY/MD
 Sample : BFB218
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB218

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 20 02:14:47 2021

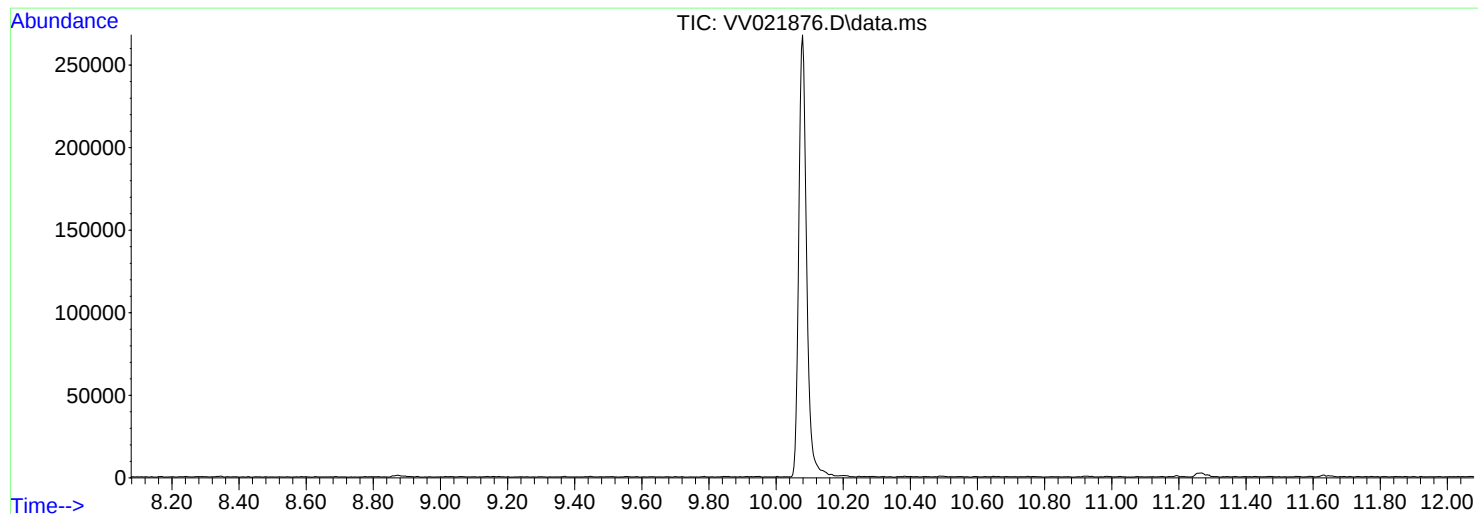

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	8553	PASS
75	95	30	80	48.5	25477	PASS
95	95	100	100	100.0	52584	PASS
96	95	5	9	7.4	3902	PASS
173	174	0.00	2	1.2	566	PASS
174	95	50	120	88.1	46307	PASS
175	174	5	9	7.7	3563	PASS
176	174	95	105	97.8	45269	PASS
177	176	5	10	6.9	3116	PASS

Scan 2799 (10.040 min): VV021876.D\data.ms
BFB218

m/z	Abundance
38.80	101.0
39.90	183.0
43.90	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
35.90	451.0
37.00	2106.0
38.00	2006.0
39.00	786.0
39.80	201.0
40.10	211.0
43.90	607.0
44.90	526.0
45.90	119.0
46.90	703.0
48.00	264.0
49.00	2013.0
50.00	8799.0
51.00	3103.0
51.90	171.0
55.00	166.0
56.00	693.0
57.00	1345.0
59.90	446.0
61.00	2460.0
62.00	2290.0
63.00	1677.0
64.00	242.0
65.00	266.0
66.80	207.0
68.00	4968.0
69.00	5048.0
70.00	433.0
72.00	404.0
73.00	2216.0
74.00	8469.0
75.00	25792.0
76.00	2248.0
76.90	322.0
77.90	335.0
78.90	1584.0
79.90	555.0
80.90	1842.0
81.90	330.0
83.00	101.0
86.00	176.0
86.90	2155.0
87.90	2169.0
90.90	275.0
92.00	1646.0
92.90	2425.0
94.00	5965.0
95.00	53328.0
96.00	3907.0
97.00	160.0
104.00	249.0
105.80	340.0
115.80	223.0
116.90	328.0
117.80	181.0
118.80	355.0
128.00	182.0
129.00	107.0
129.90	172.0
134.80	155.0
140.80	629.0
142.90	755.0
147.80	194.0
154.80	140.0
171.70	280.0
173.00	542.0
173.90	44944.0
175.00	3433.0
175.90	44248.0
176.90	3141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	417.0
37.00	2229.0
38.00	2076.0
39.00	826.0
39.80	171.0
43.90	658.0
44.90	480.0
45.90	120.0
46.90	775.0
48.00	297.0
49.00	1938.0
50.00	8855.0
51.00	3109.0
51.90	167.0
53.00	112.0
55.00	181.0
56.00	721.0
57.00	1406.0
58.10	106.0
59.90	444.0
61.00	2565.0
62.00	2451.0
63.00	1685.0
64.00	252.0
65.00	303.0
66.80	169.0
68.00	5144.0
69.00	5178.0
70.00	442.0
71.90	318.0
73.00	2219.0
74.00	8378.0
75.00	26320.0
76.00	2255.0
77.00	290.0
78.00	287.0
78.90	1573.0
79.90	561.0
80.90	1798.0
81.90	388.0
86.00	164.0
86.90	2176.0
87.90	2358.0
90.90	200.0
92.00	1626.0
92.90	2450.0
94.00	5950.0
95.00	54248.0
96.00	4076.0
97.00	188.0
103.90	309.0
105.80	273.0
115.80	244.0
116.90	329.0
117.80	203.0
118.80	362.0
127.90	219.0
129.00	137.0
129.90	199.0
134.90	132.0
140.80	702.0
142.90	766.0
147.80	194.0
154.80	133.0
156.80	111.0
171.80	302.0
172.30	284.0
172.90	582.0
173.90	47832.0
175.00	3743.0
175.90	46864.0
176.90	3223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218

m/z	Abundance
36.00	452.0
37.00	2182.0
38.00	1927.0
39.00	833.0
39.90	182.0
43.90	671.0
44.90	403.0
45.90	115.0
46.90	819.0
48.00	263.0
49.00	1732.0
50.00	8005.0
51.00	2810.0
52.00	138.0
53.00	109.0
55.00	159.0
55.90	680.0
57.00	1291.0
58.10	102.0
60.00	416.0
61.00	2397.0
62.00	2335.0
62.90	1611.0
64.00	234.0
65.00	307.0
66.80	118.0
68.00	4668.0
69.00	4831.0
69.90	496.0
72.00	225.0
73.00	2035.0
74.00	7746.0
75.00	24320.0
76.00	2028.0
77.10	296.0
78.00	240.0
78.90	1460.0
79.90	551.0
80.90	1652.0
81.90	421.0
86.00	125.0
86.90	2082.0
87.90	2316.0
90.80	186.0
92.00	1426.0
92.90	2140.0
94.00	5403.0
95.00	50176.0
96.00	3723.0
97.00	163.0
103.90	313.0
104.90	107.0
105.80	222.0
115.80	244.0
116.80	300.0
117.80	209.0
118.80	320.0
127.90	241.0
128.90	170.0
129.90	234.0
140.80	676.0
142.00	108.0
142.80	707.0
147.80	181.0
154.70	122.0
172.00	323.0
172.90	574.0
174.00	46144.0
175.00	3514.0
175.90	44696.0
177.00	2983.0

Instrument :
MSVOA_V
ClientSampleId :
BFB218