




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027444.D
Acq On : 19 Aug 2022 16:44
Operator : SY/MD
Sample : N4253-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 06:06:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 20 05:55:43 2022
Response via : Initial Calibration

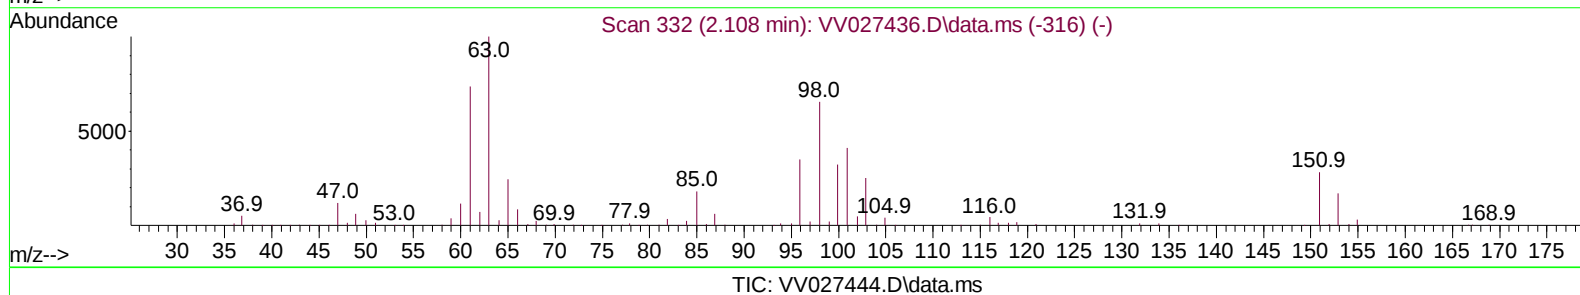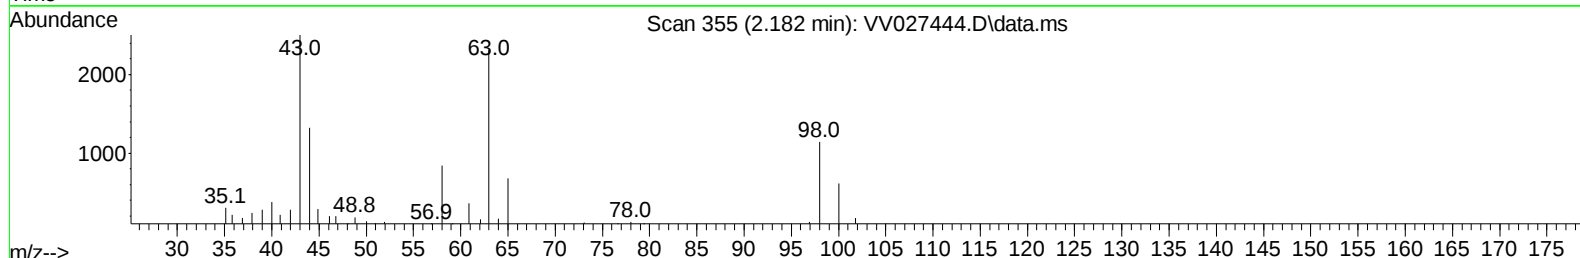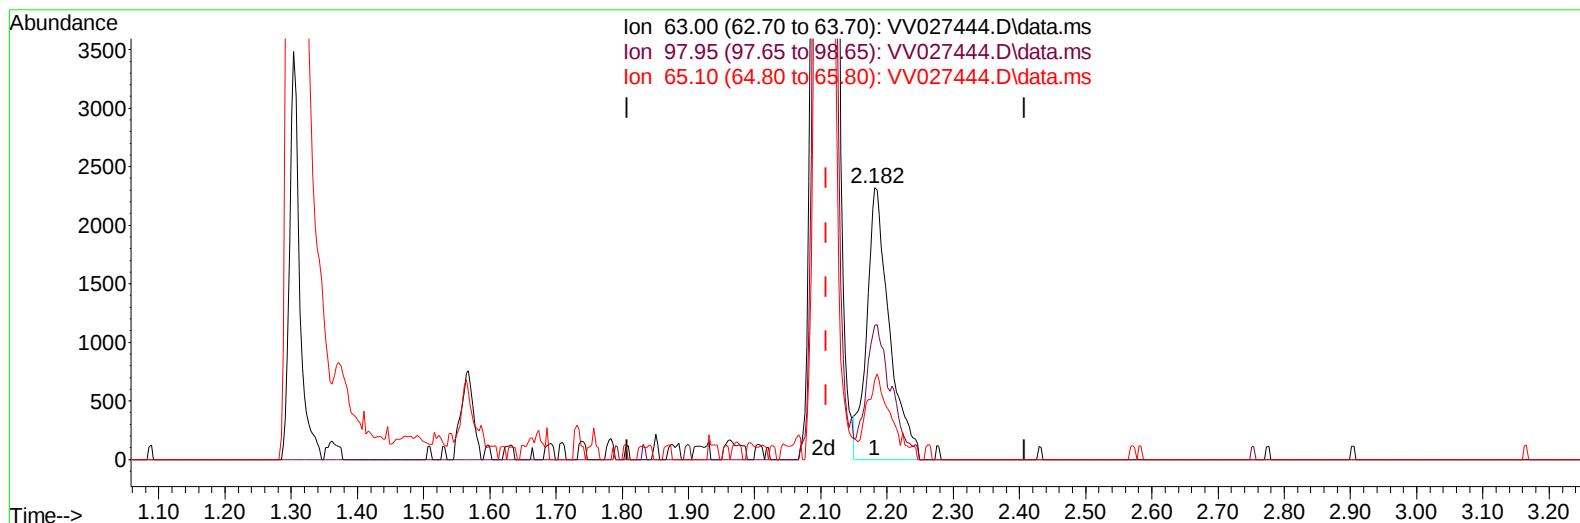

(11) 1,1-Dichloroethene-d2 (S)

2.182min (+ 0.074) 0.25 ug/L

response 5469

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	55.33
65.10	22.40	23.97
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027444.D
 Acq On : 19 Aug 2022 16:44
 Operator : SY/MD
 Sample : N4253-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D8

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:06:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

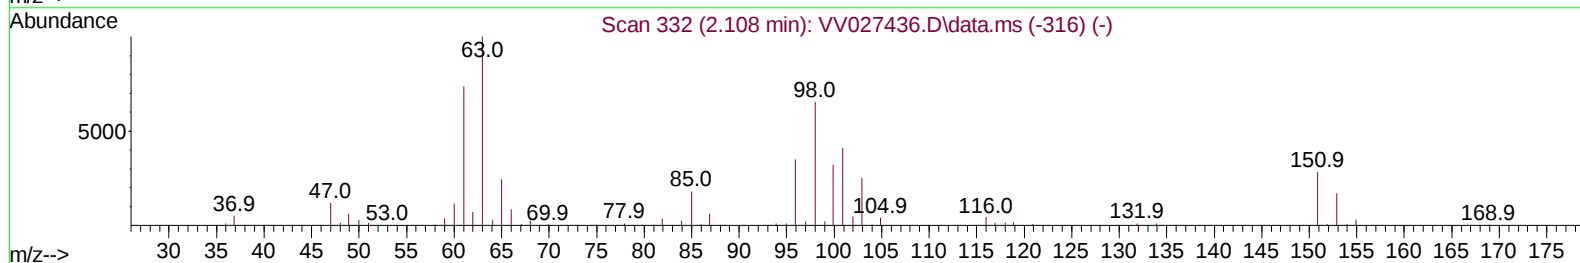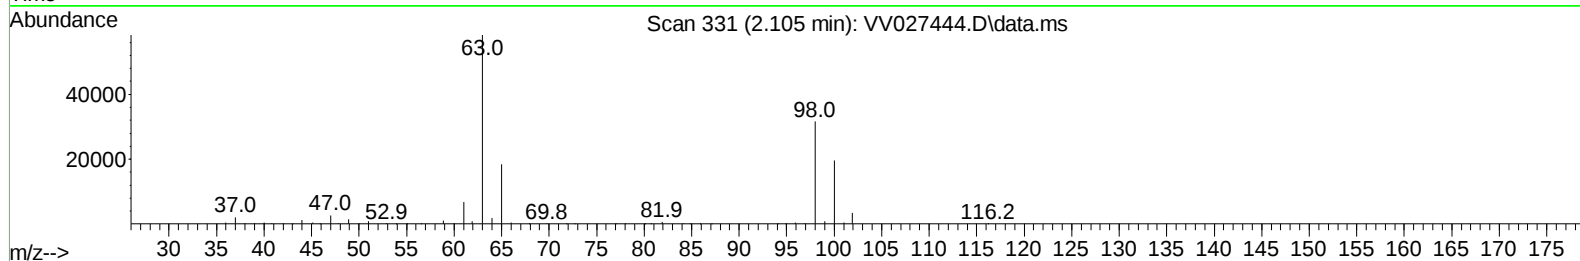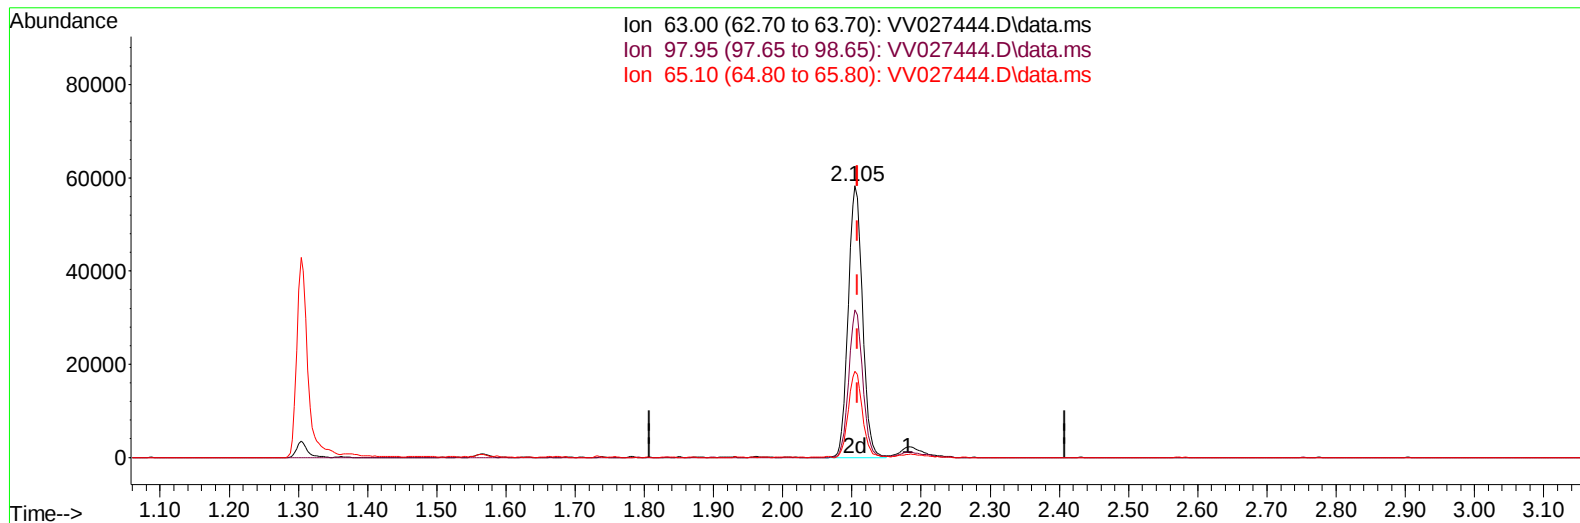

TIC: VV027444.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (-0.003) 3.82 ug/L m

response 82964

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	3.65#
65.10	22.40	1.58#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027444.D
 Acq On : 19 Aug 2022 16:44
 Operator : SY/MD
 Sample : N4253-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 06:06:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		130916	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		134832	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		58425	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		47916	5.143	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	102.800%	
7) Chloroethane-d5	1.564	69		44934	6.589	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	131.800%#	
11) 1,1-Dichloroethene-d2	2.105	63		82964m	3.819	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	76.400%	
20) 2-Butanone-d5	3.892	46		78006	67.273	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	134.540%#	
24) Chloroform-d	4.346	84		89469	4.802	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	96.000%	
26) 1,2-Dichloroethane-d4	5.034	65		46171	5.729	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	114.600%	
32) Benzene-d6	5.050	84		187434	5.019	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	100.400%	
36) 1,2-Dichloropropane-d6	6.069	67		57355	5.282	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	105.600%	
41) Toluene-d8	7.317	98		148131	4.393	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	87.800%	
43) trans-1,3-Dichloroprop...	7.625	79		16900	4.546	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	91.000%	
46) 2-Hexanone-d5	8.088	63		55121	45.041	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	90.080%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		33418	4.833	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	96.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152		45296	5.230	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	104.600%	
Target Compounds							
13) Acetone	2.169	43		5981	5.401	ug/L	Qvalue 81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027444.D
Acq On : 19 Aug 2022 16:44
Operator : SY/MD
Sample : N4253-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D8

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:06:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 20 05:55:43 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022

