




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027448.D
 Acq On : 19 Aug 2022 18:22
 Operator : SY/MD
 Sample : N4253-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:07:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

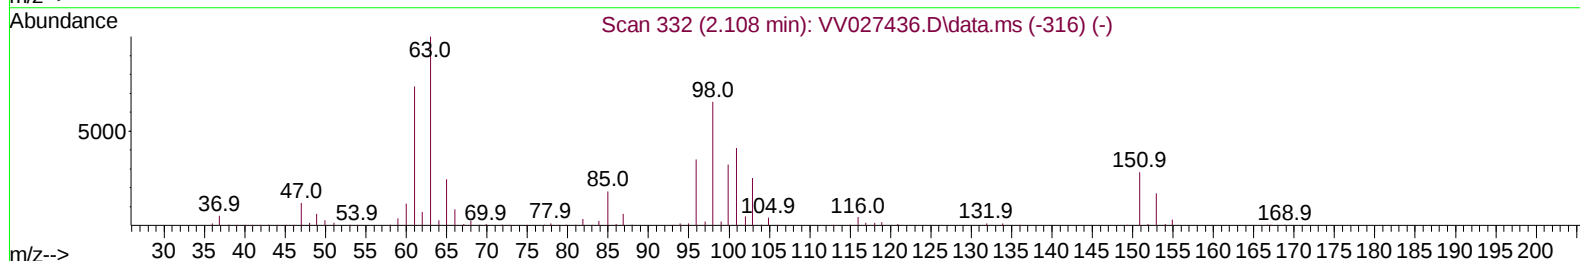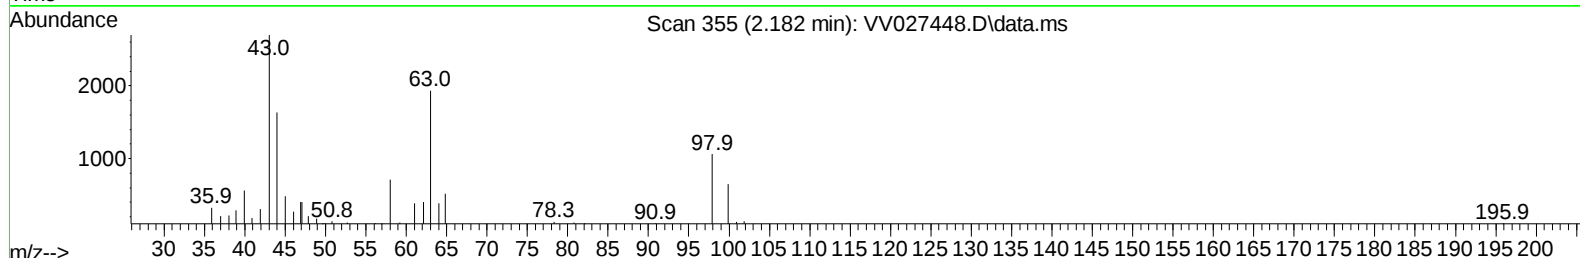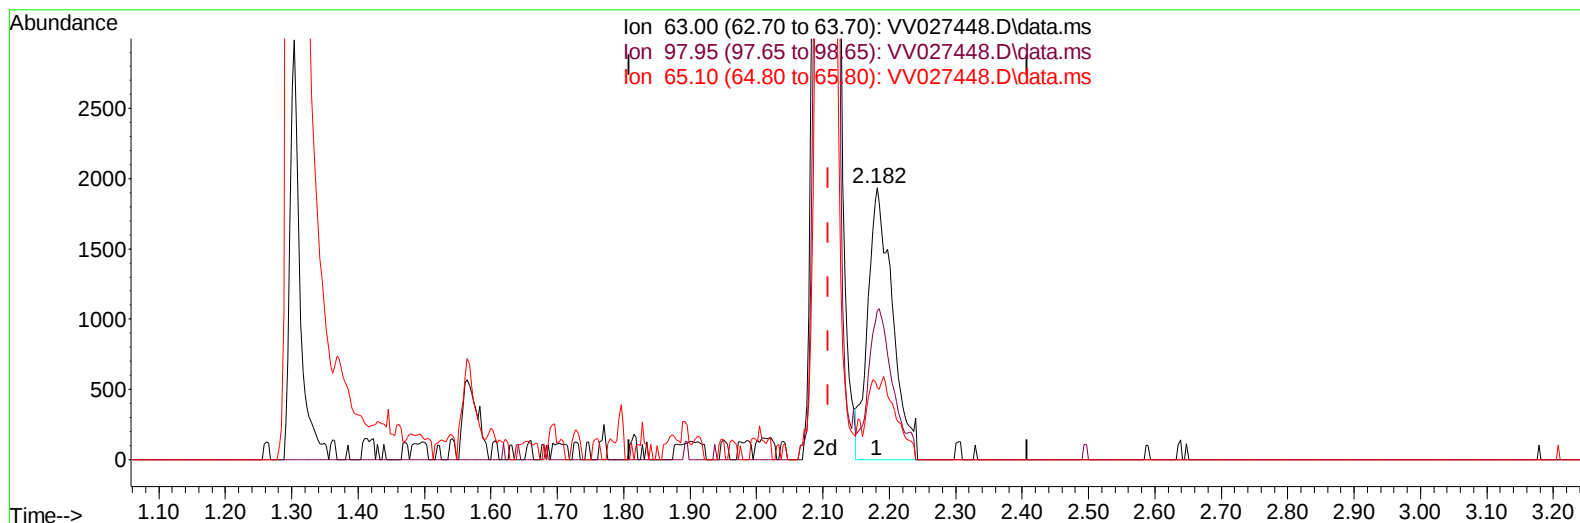

TIC: VV027448.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.182min (+ 0.074) 0.24 ug/L

response 4953

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	54.39
65.10	22.40	19.50
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027448.D
 Acq On : 19 Aug 2022 18:22
 Operator : SY/MD
 Sample : N4253-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:07:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

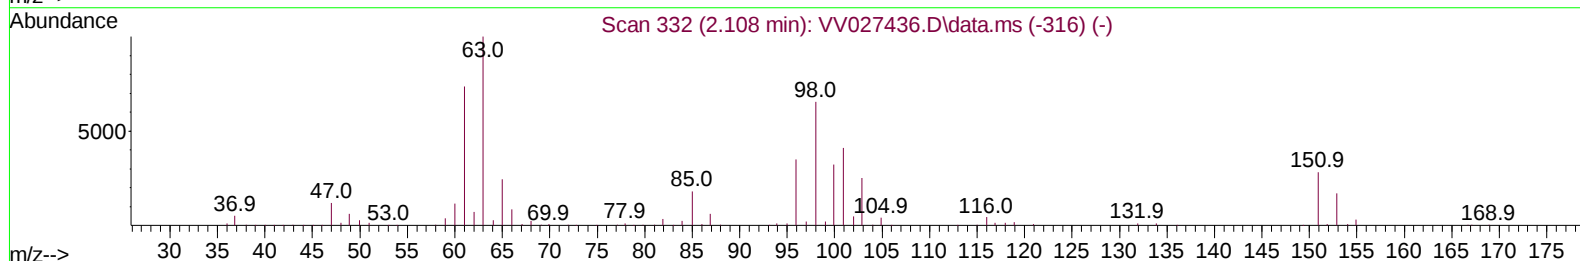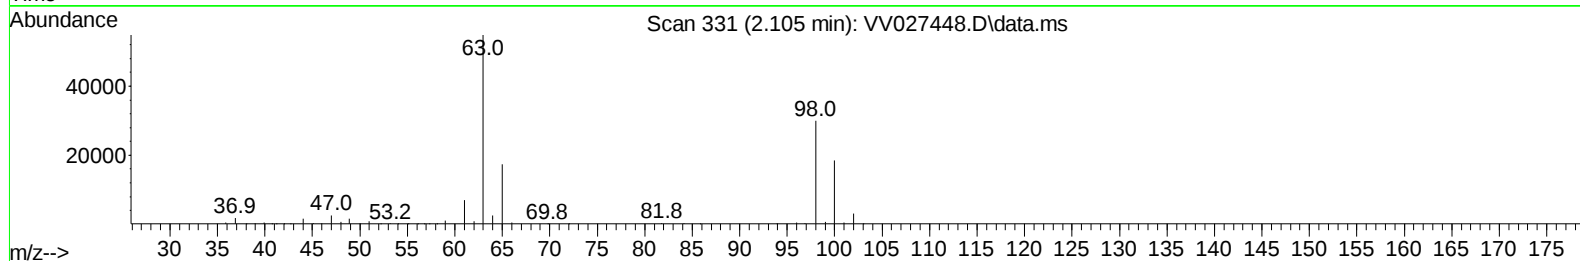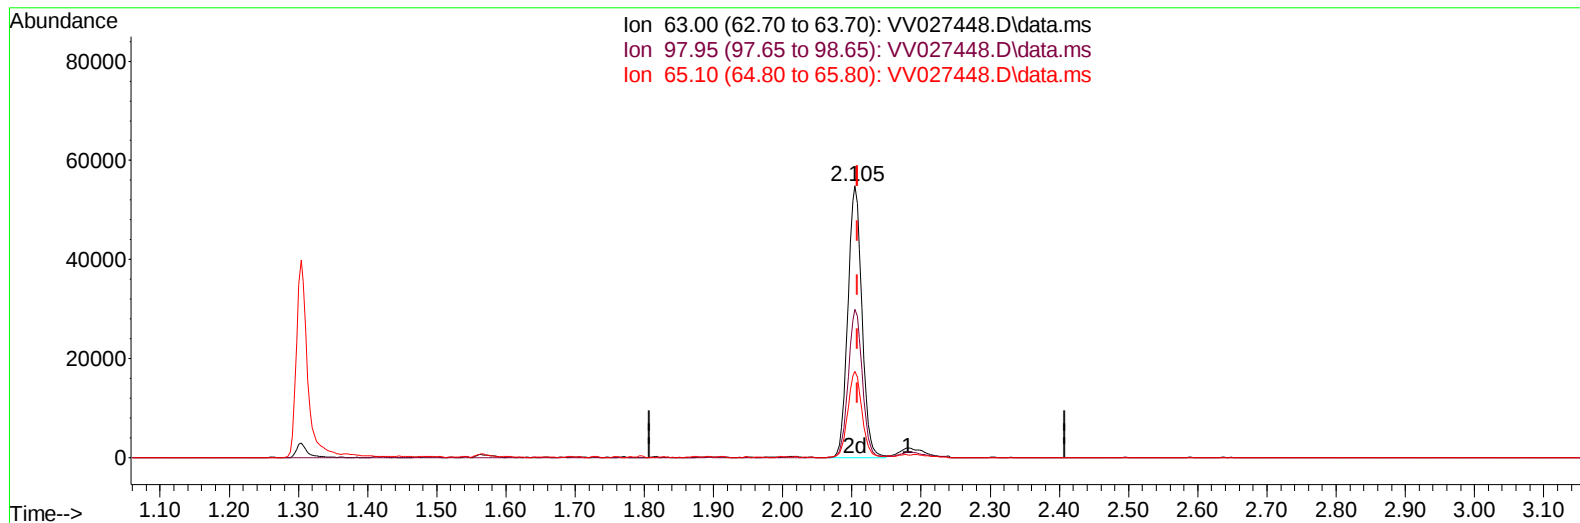

TIC: VV027448.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (-0.003) 3.66 ug/L m

response 76708

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	3.51#
65.10	22.40	1.26#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027448.D
 Acq On : 19 Aug 2022 18:22
 Operator : SY/MD
 Sample : N4253-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:07:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

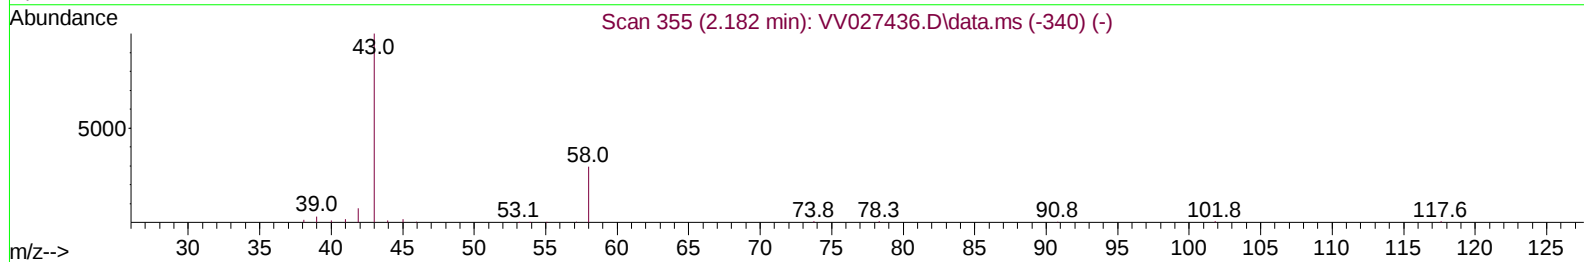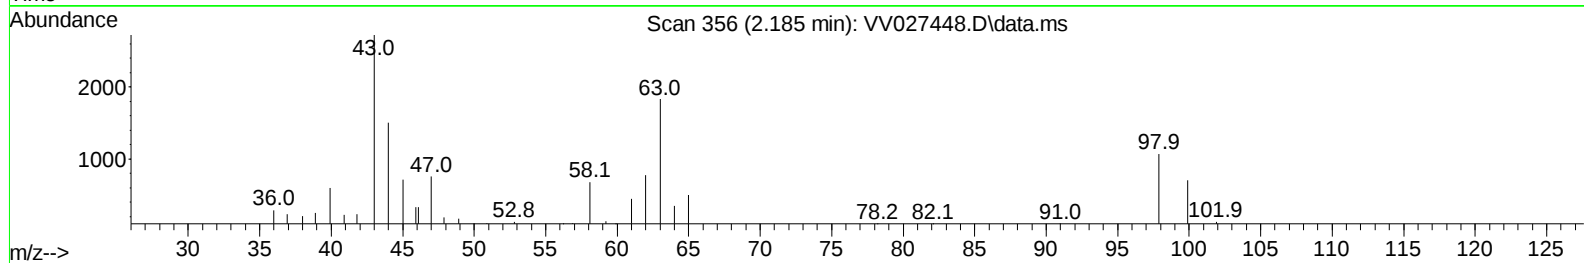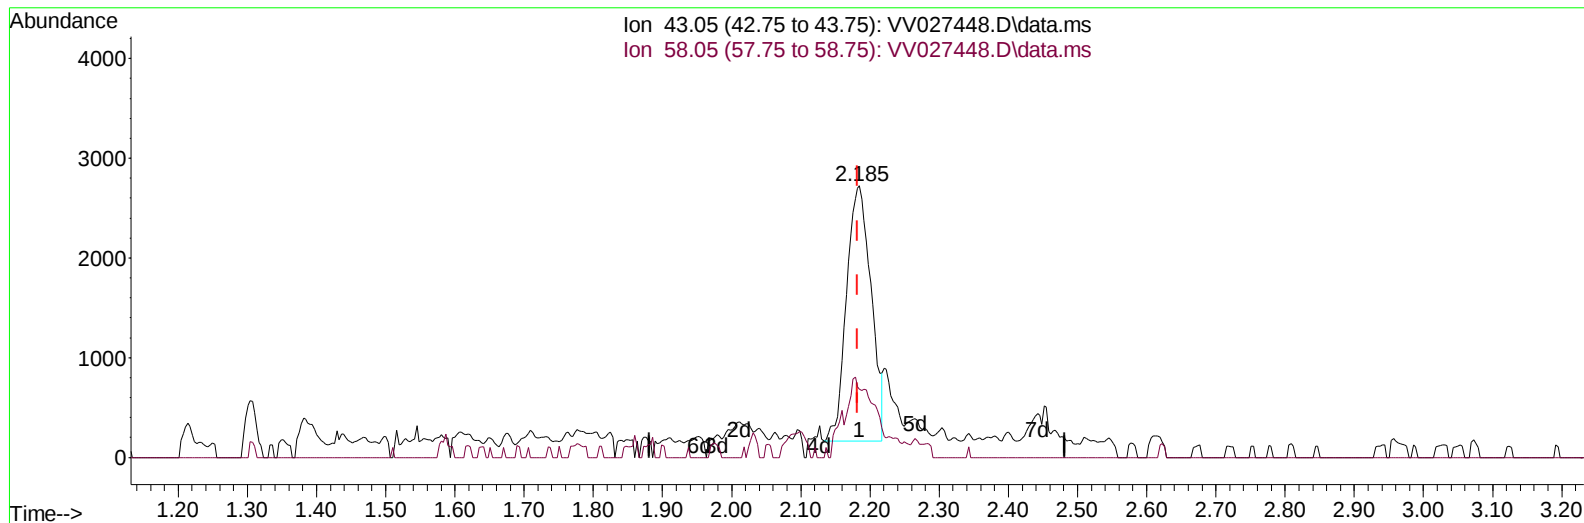

TIC: VV027448.D\data.ms

(13) Acetone (T)

2.185min (+ 0.003) 5.95 ug/L

response 6356

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	30.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027448.D
 Acq On : 19 Aug 2022 18:22
 Operator : SY/MD
 Sample : N4253-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:07:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

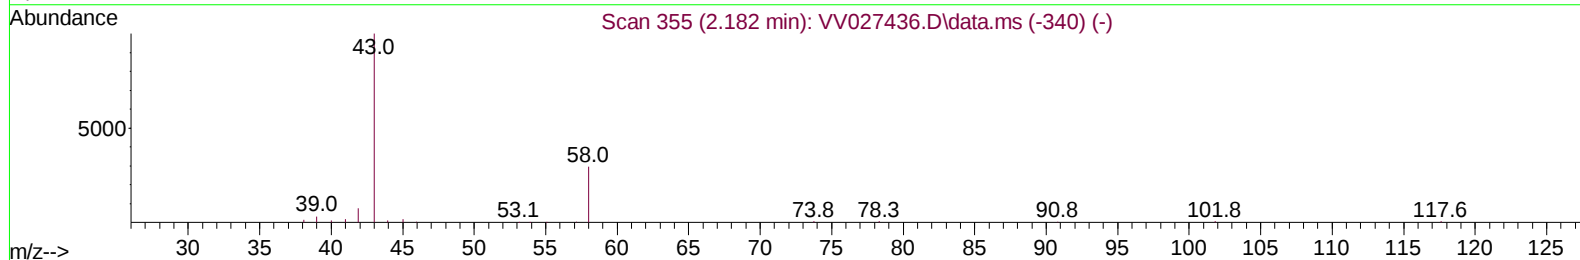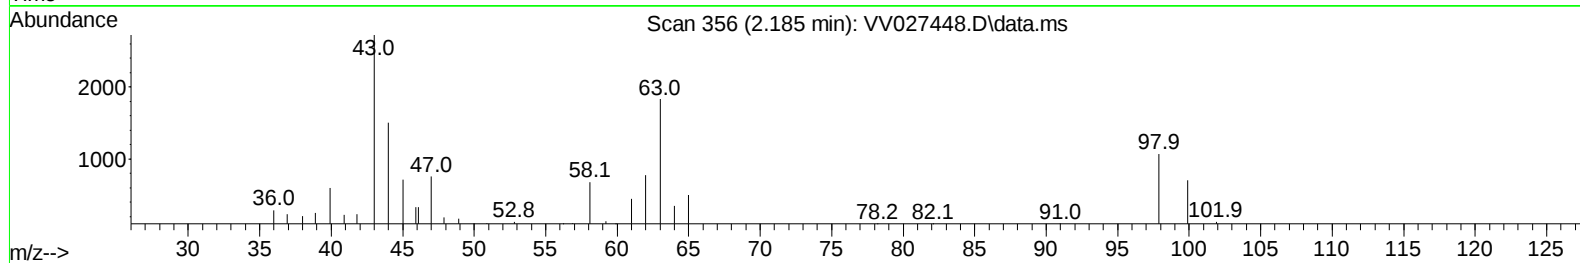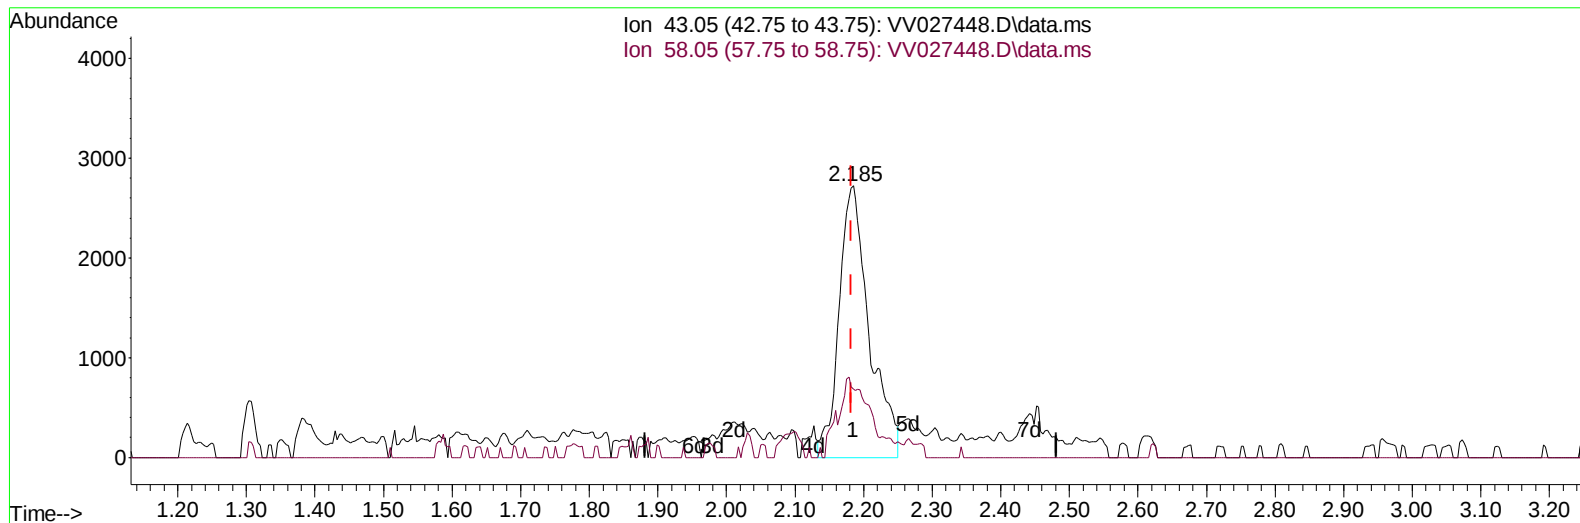

TIC: VV027448.D\data.ms

(13) Acetone (T)

2.185min (+ 0.003) 7.76 ug/L m

response 8295

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	23.45
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027448.D
 Acq On : 19 Aug 2022 18:22
 Operator : SY/MD
 Sample : N4253-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:07:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		126295	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		124327	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		53794	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		44407	4.940	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.800%	
7) Chloroethane-d5	1.564	69		41784	6.352	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	127.000%	
11) 1,1-Dichloroethene-d2	2.105	63		76708m	3.660	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%	
20) 2-Butanone-d5	3.896	46		69999	62.577	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.160%	
24) Chloroform-d	4.346	84		86785	4.829	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.600%	
26) 1,2-Dichloroethane-d4	5.034	65		39216	5.044	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%	
32) Benzene-d6	5.047	84		168135	4.882	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%	
36) 1,2-Dichloropropane-d6	6.069	67		51820	5.176	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.600%	
41) Toluene-d8	7.313	98		133041	4.279	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.625	79		15487	4.518	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.091	63		48593	43.062	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.120%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		30645	4.806	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		41847	5.248	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.000%	
Target Compounds							
13) Acetone	2.185	43		8295m	7.765	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027448.D
Acq On : 19 Aug 2022 18:22
Operator : SY/MD
Sample : N4253-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9E2

Manual IntegrationsAPPROVED

Quant Time: Aug 20 06:07:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 20 05:55:43 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022

