

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027445.D
 Acq On : 19 Aug 2022 17:08
 Operator : SY/MD
 Sample : N4253-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D9

Quant Time: Aug 20 06:06:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	123846	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	126161	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53761	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	45189	5.127	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 102.600%		
7) Chloroethane-d5	1.565	69	42622	6.607	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 132.200%#		
11) 1,1-Dichloroethene-d2	2.105	63	77257	3.759	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 75.200%		
20) 2-Butanone-d5	3.896	46	71729	65.391	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 130.780%#		
24) Chloroform-d	4.346	84	86151	4.888	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 97.800%		
26) 1,2-Dichloroethane-d4	5.034	65	41559	5.451	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 109.000%		
32) Benzene-d6	5.047	84	169027	4.837	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 96.800%		
36) 1,2-Dichloropropane-d6	6.066	67	51717	5.090	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 101.800%		
41) Toluene-d8	7.314	98	137193	4.348	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 87.000%		
43) trans-1,3-Dichloroprop...	7.625	79	16069	4.619	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 92.400%		
46) 2-Hexanone-d5	8.088	63	50285	43.914	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 87.820%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31537	4.874	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 97.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	42421	5.323	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 106.400%		
Target Compounds						
13) Acetone	2.185	43	7356	7.022	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027445.D
Acq On : 19 Aug 2022 17:08
Operator : SY/MD
Sample : N4253-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D9

Quant Time: Aug 20 06:06:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 20 05:55:43 2022
Response via : Initial Calibration

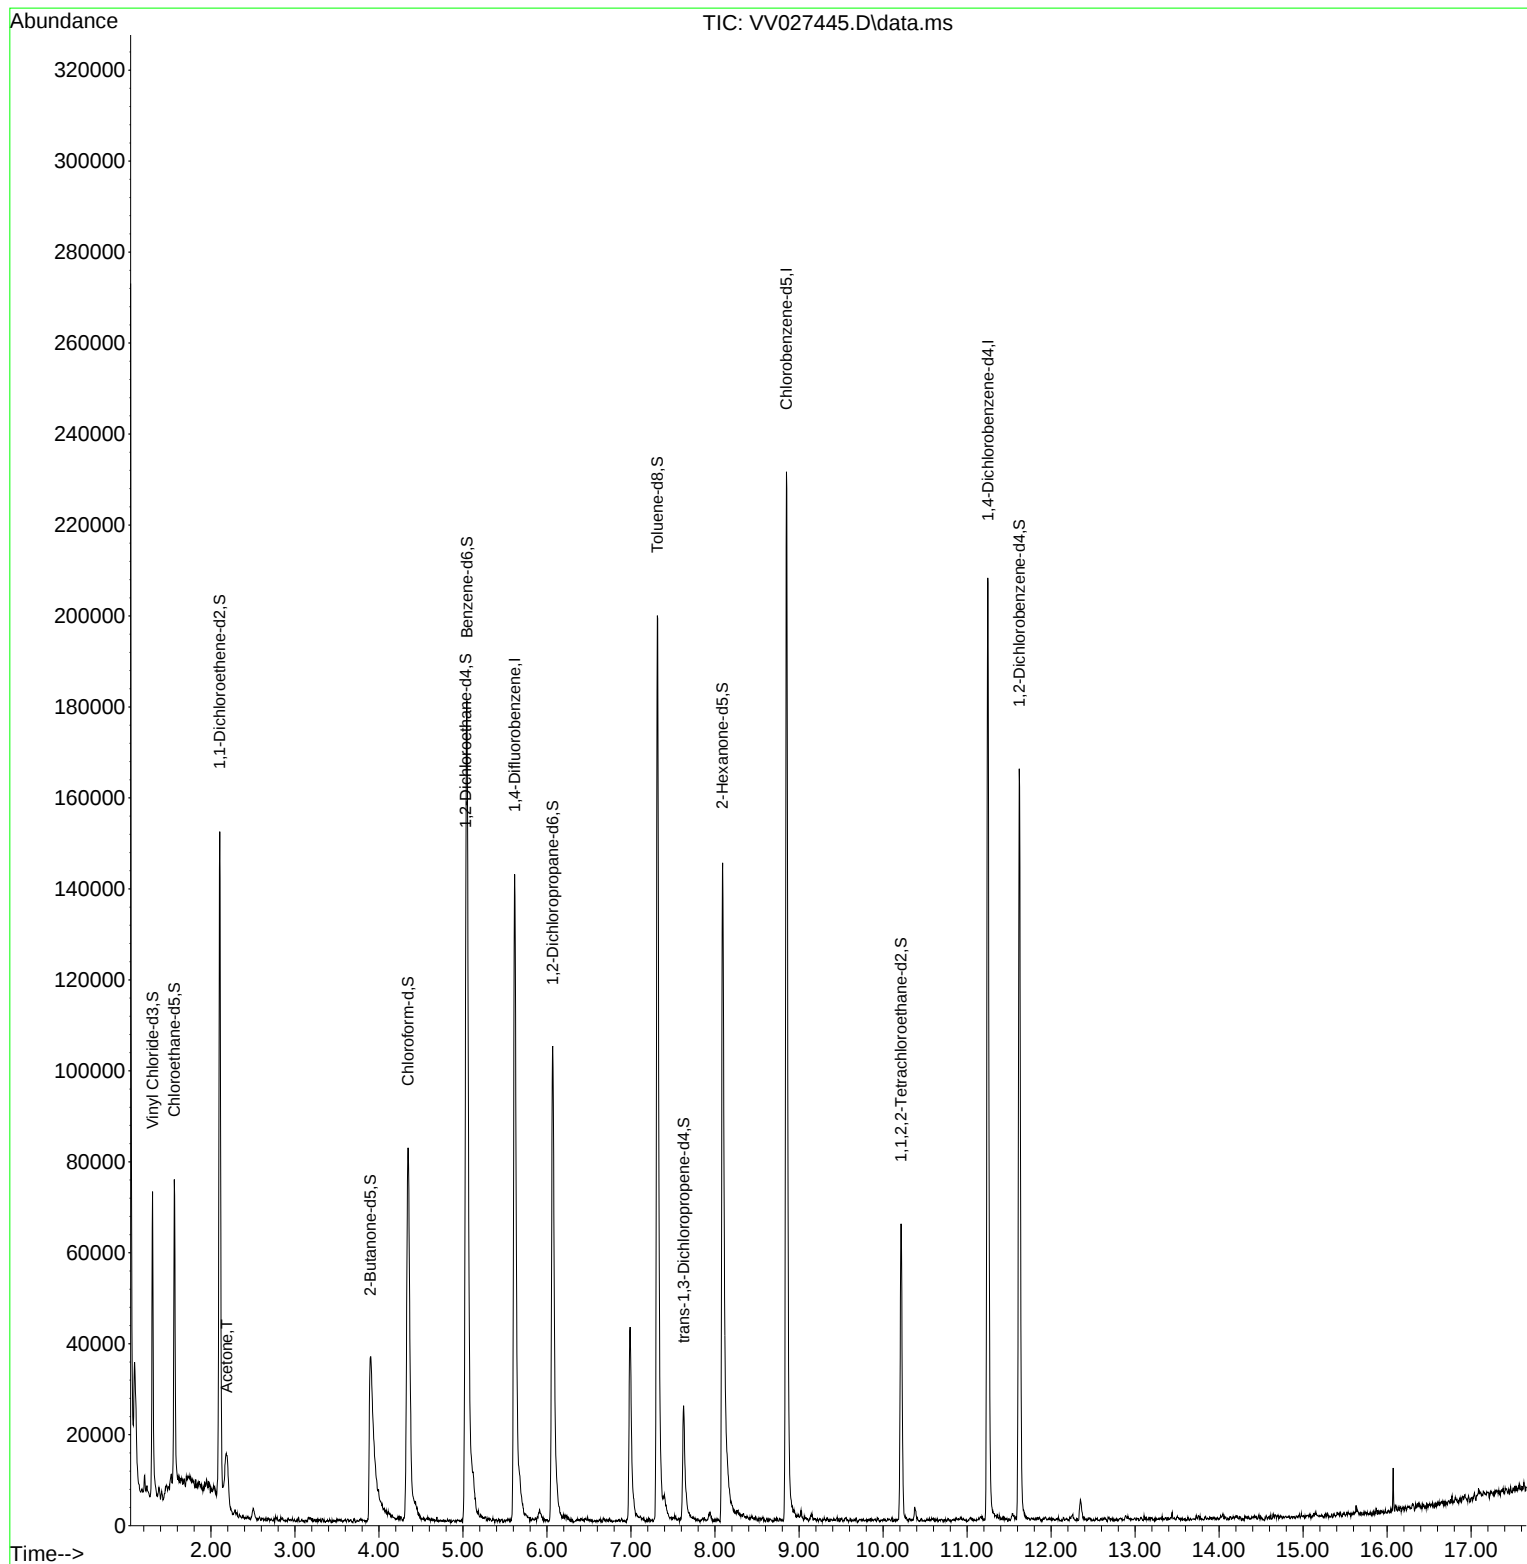

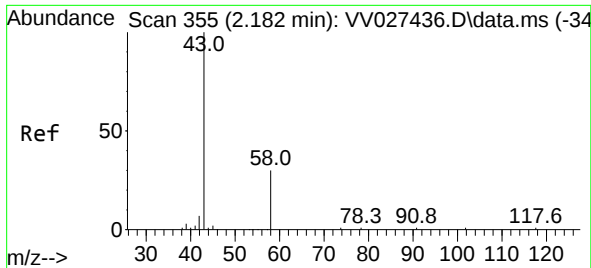

#13
 Acetone
 Concen: 7.022 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV027445.D
 Acq: 19 Aug 2022 17:08

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D9

Tgt Ion: 43 Resp: 7356
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 62.2

