

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027448.D
 Acq On : 19 Aug 2022 18:22
 Operator : SY/MD
 Sample : N4253-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

Quant Time: Aug 20 06:07:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 20 05:55:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	126295	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	124327	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53794	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44407	4.940	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	98.800%	
7) Chloroethane-d5	1.564	69	41784	6.352	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	127.000%	
11) 1,1-Dichloroethene-d2	2.105	63	76708m	3.660	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	73.200%	
20) 2-Butanone-d5	3.896	46	69999	62.577	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	125.160%	
24) Chloroform-d	4.346	84	86785	4.829	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.600%	
26) 1,2-Dichloroethane-d4	5.034	65	39216	5.044	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.800%	
32) Benzene-d6	5.047	84	168135	4.882	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
36) 1,2-Dichloropropane-d6	6.069	67	51820	5.176	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.600%	
41) Toluene-d8	7.313	98	133041	4.279	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.625	79	15487	4.518	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.091	63	48593	43.062	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	86.120%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30645	4.806	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	41847	5.248	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.000%	
Target Compounds					Qvalue	
13) Acetone	2.185	43	8295m	7.765	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027448.D
Acq On : 19 Aug 2022 18:22
Operator : SY/MD
Sample : N4253-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
EX9E2

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 08/22/2022
Supervised By :Mahesh Dadoda 08/22/2022


Quant Time: Aug 20 06:07:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 20 05:55:43 2022
Response via : Initial Calibration

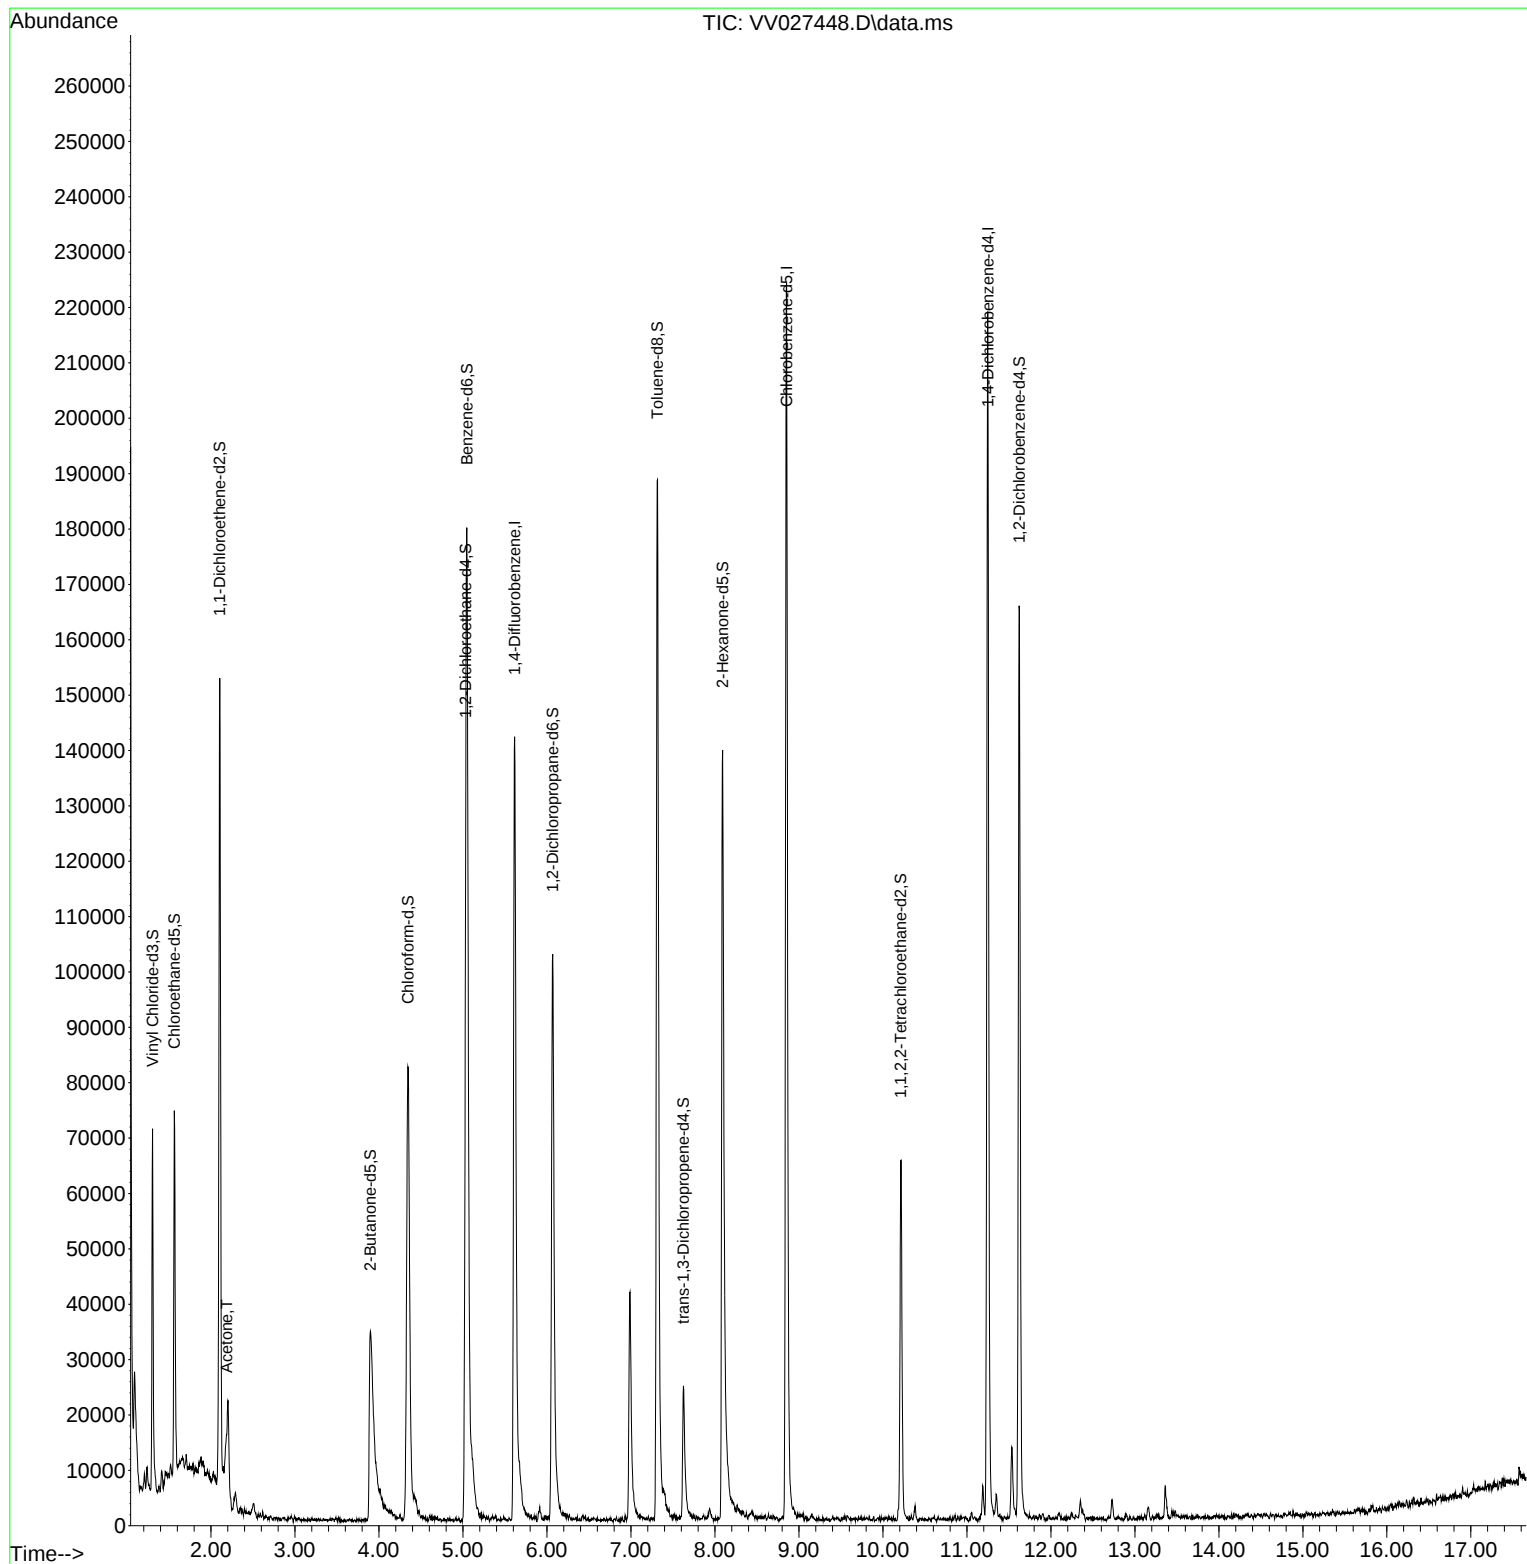

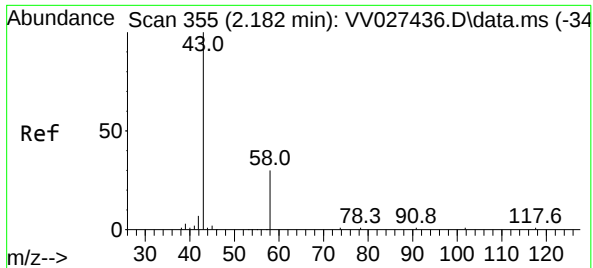

#13
 Acetone
 Concen: 7.765 ug/L m
 RT: 2.185 min Scan# 3
 Delta R.T. 0.003 min
 Lab File: VV027448.D
 Acq: 19 Aug 2022 18:22

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E2

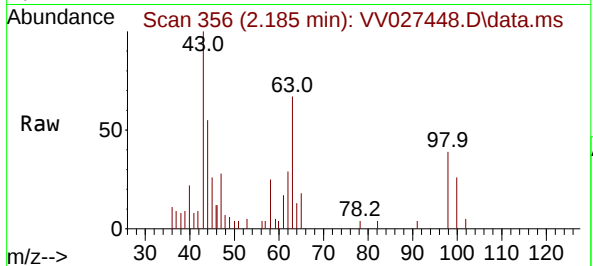

Tgt Ion: 43 Resp: 829
 Ion Ratio Lower Upper
 43 100
 58 23.4 0.0 62.2

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 08/22/2022
 Supervised By :Mahesh Dadoda 08/22/2022

