

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027445.D
 Acq On : 19 Aug 2022 17:08
 Operator : SY/MD
 Sample : N4253-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.092	11	16	38	rVB	28530	57360	12.32%	1.534%
2	1.304	74	82	99	rVB	66970	73983	15.89%	1.978%
3	1.565	156	163	175	rVV	66676	78091	16.77%	2.088%
4	2.105	319	331	341	rBV	146047	208559	44.79%	5.577%
5	2.182	348	355	357	rBV6	5839	7751	1.66%	0.207%
6	2.503	446	455	468	rVB8	2547	4956	1.06%	0.133%
7	3.899	876	889	916	rBV	36232	134372	28.86%	3.593%
8	4.346	1014	1028	1054	rBV	81431	217186	46.64%	5.807%
9	5.047	1230	1246	1268	rBV2	180674	465661	100.00%	12.451%
10	5.616	1409	1423	1458	rBV	142182	317735	68.23%	8.496%
11	6.069	1548	1564	1597	rBV	104590	238181	51.15%	6.369%
12	6.989	1835	1850	1871	rBV2	42879	88513	19.01%	2.367%
13	7.314	1935	1951	1970	rBV	199204	364751	78.33%	9.753%
14	7.625	2038	2048	2067	rBV2	25040	50945	10.94%	1.362%
15	8.092	2183	2193	2223	rBV	144928	317886	68.27%	8.500%
16	8.850	2418	2429	2449	rBV	230673	393065	84.41%	10.510%
17	10.214	2843	2853	2869	rBV	64991	105232	22.60%	2.814%
18	11.246	3163	3174	3192	rBV	207165	333295	71.57%	8.912%
19	11.622	3281	3291	3310	rBV	165147	268770	57.72%	7.187%
20	12.349	3508	3517	3527	rBV9	4632	8215	1.76%	0.220%
21	16.072	4672	4675	4680	rVB	9461	5346	1.15%	0.143%




Sum of corrected areas: 3739853

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027445.D
Acq On : 19 Aug 2022 17:08
Operator : SY/MD
Sample : N4253-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

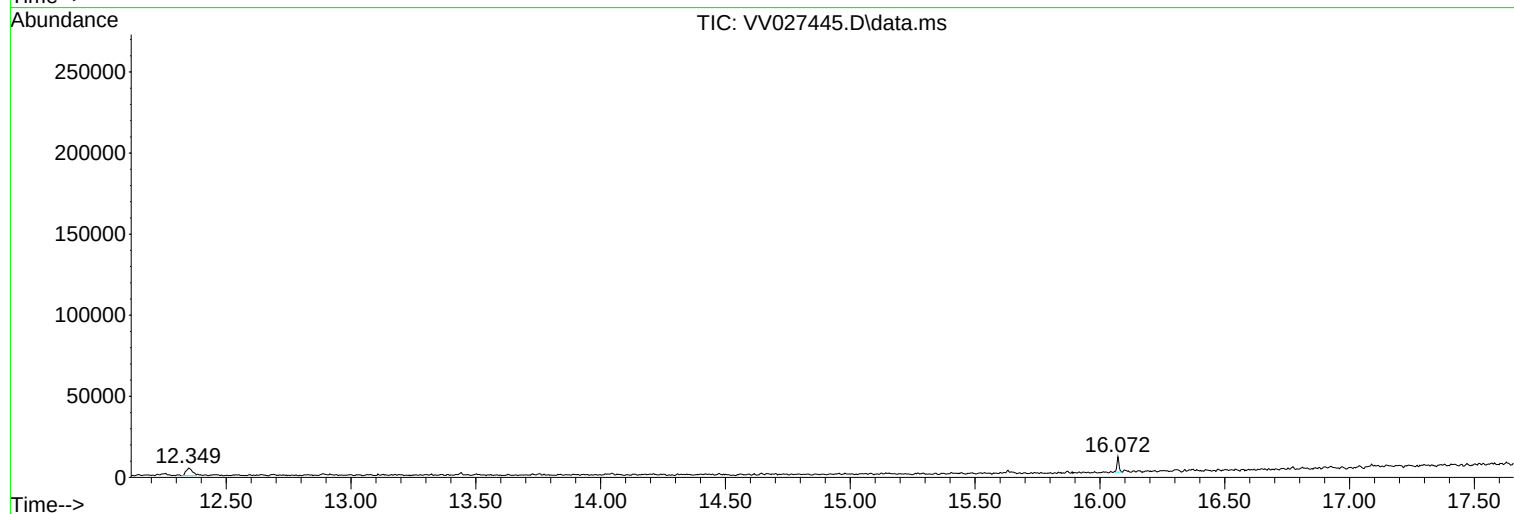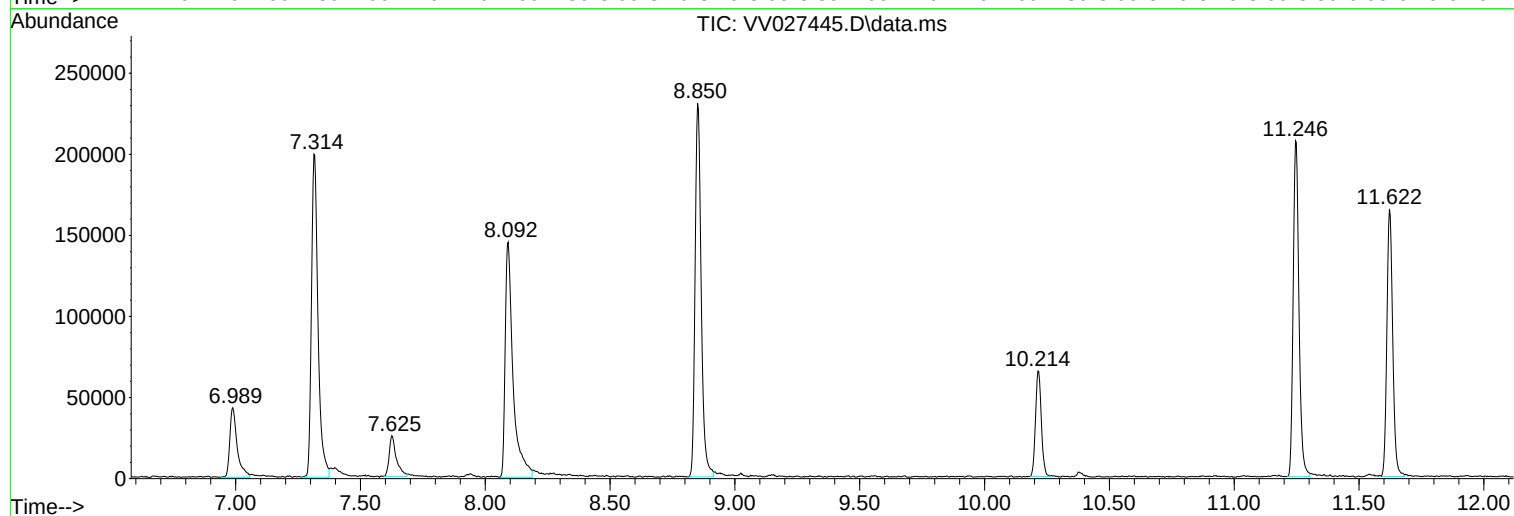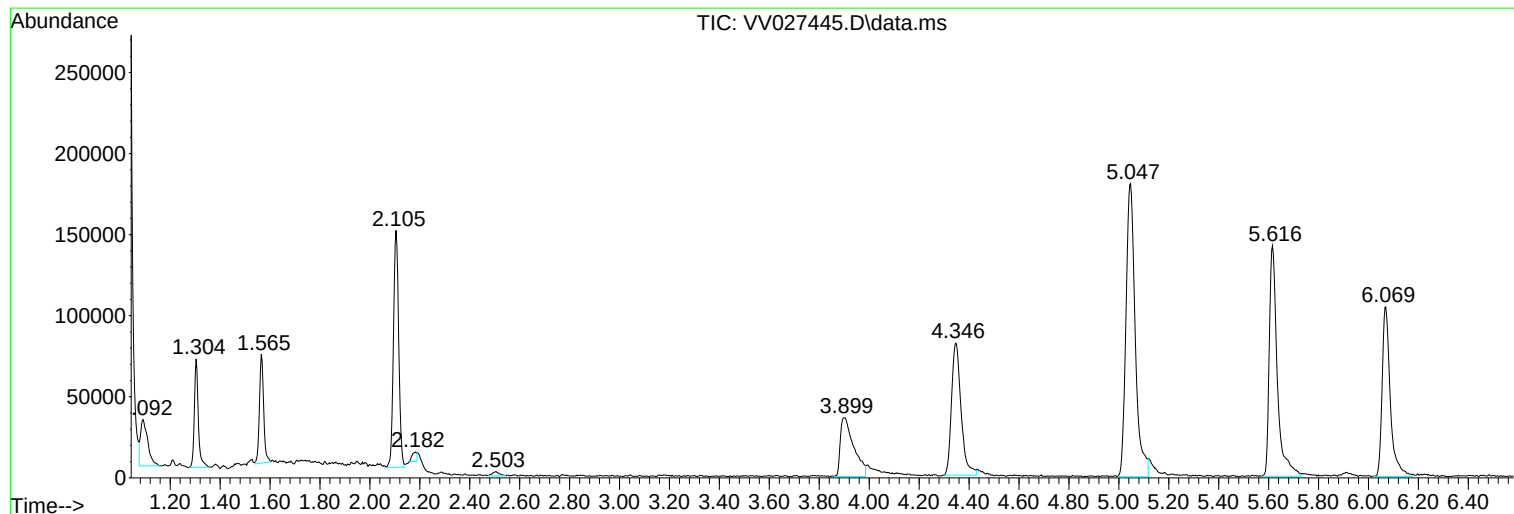

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027445.D
Acq On : 19 Aug 2022 17:08
Operator : SY/MD
Sample : N4253-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027445.D
Acq On : 19 Aug 2022 17:08
Operator : SY/MD
Sample : N4253-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc