

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027447.D
 Acq On : 19 Aug 2022 17:58
 Operator : SY/MD
 Sample : N4253-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9E1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	19	rBV	9272	8085	1.72%	0.222%
2	1.304	74	82	91	rBV	68346	75231	15.97%	2.068%
3	1.564	157	163	173	rBV	65217	73777	15.66%	2.028%
4	2.105	321	331	345	rBV	139087	205199	43.56%	5.641%
5	2.179	345	354	373	rVB	8844	28277	6.00%	0.777%
6	3.889	878	886	924	rBV	36310	129459	27.48%	3.559%
7	4.346	1008	1028	1055	rBV2	82196	219566	46.61%	6.036%
8	5.043	1227	1245	1288	rBV3	176788	471085	100.00%	12.949%
9	5.616	1410	1423	1458	rBV2	141865	318927	67.70%	8.767%
10	6.069	1552	1564	1587	rBV	102032	227330	48.26%	6.249%
11	6.989	1839	1850	1869	rBV	41712	84030	17.84%	2.310%
12	7.317	1940	1952	1975	rBV	188511	356323	75.64%	9.795%
13	7.625	2035	2048	2064	rBV2	24036	48398	10.27%	1.330%
14	8.091	2183	2193	2226	rBV	142183	306932	65.15%	8.437%
15	8.850	2418	2429	2453	rBV	222465	382994	81.30%	10.528%
16	10.217	2843	2854	2872	rVB	64057	103923	22.06%	2.857%
17	10.381	2898	2905	2917	rVB4	3552	6000	1.27%	0.165%
18	11.249	3164	3175	3196	rBV	205273	331786	70.43%	9.120%
19	11.622	3281	3291	3313	rBV	157851	260574	55.31%	7.163%




Sum of corrected areas: 3637896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027447.D
Acq On : 19 Aug 2022 17:58
Operator : SY/MD
Sample : N4253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

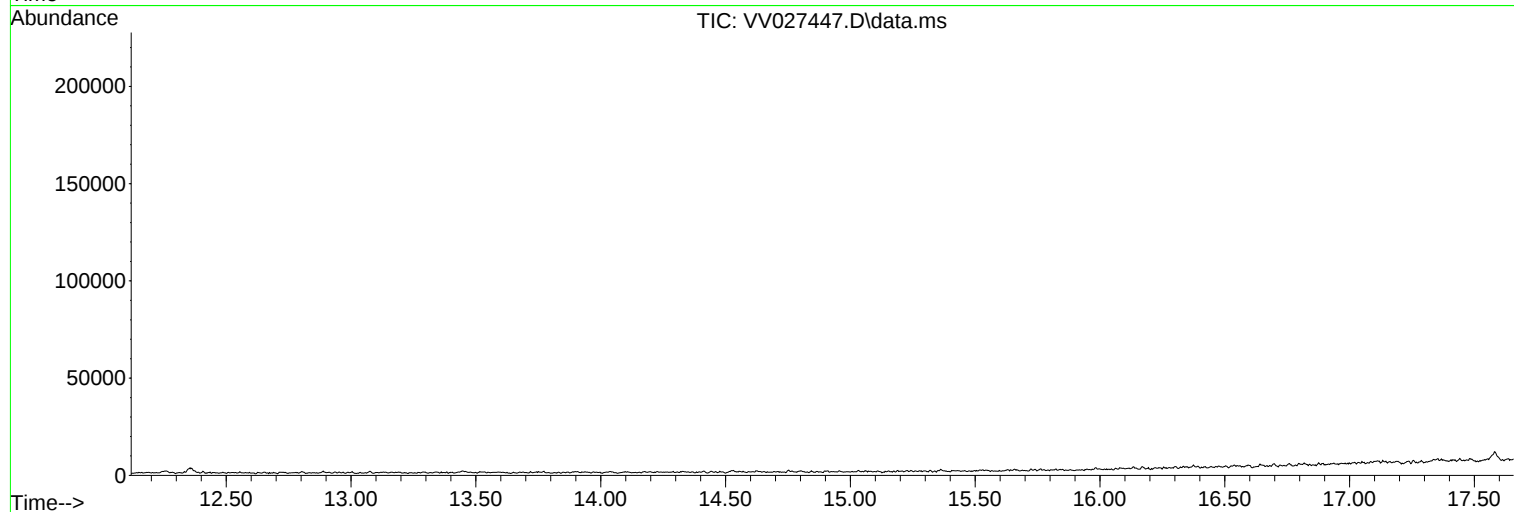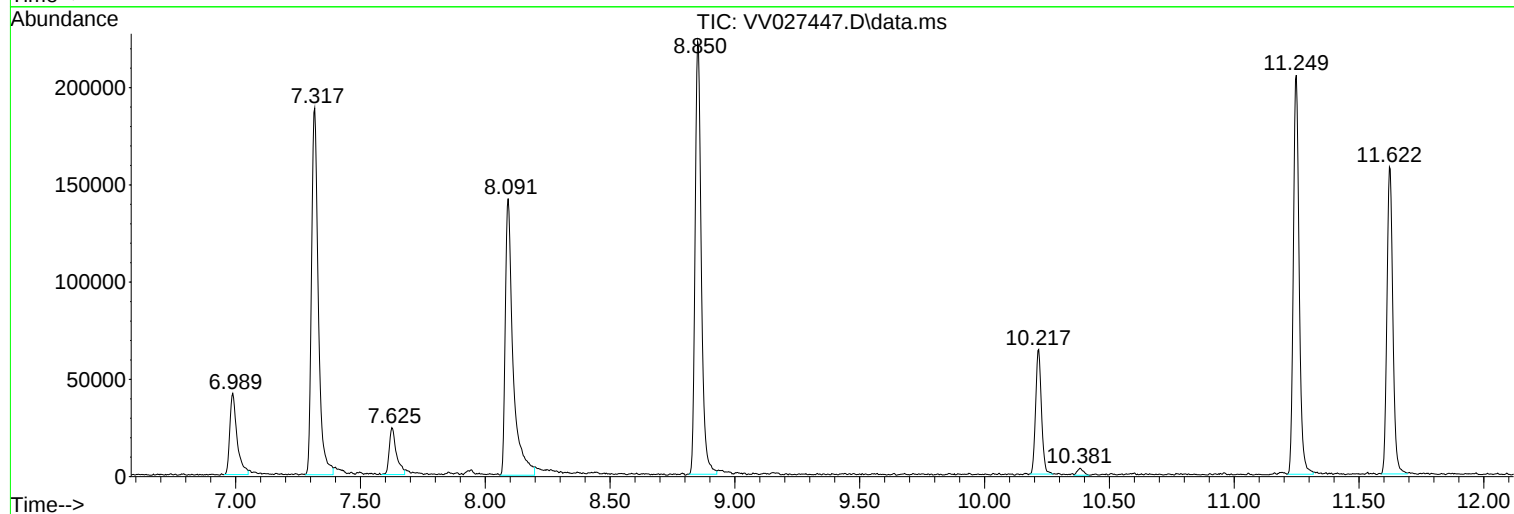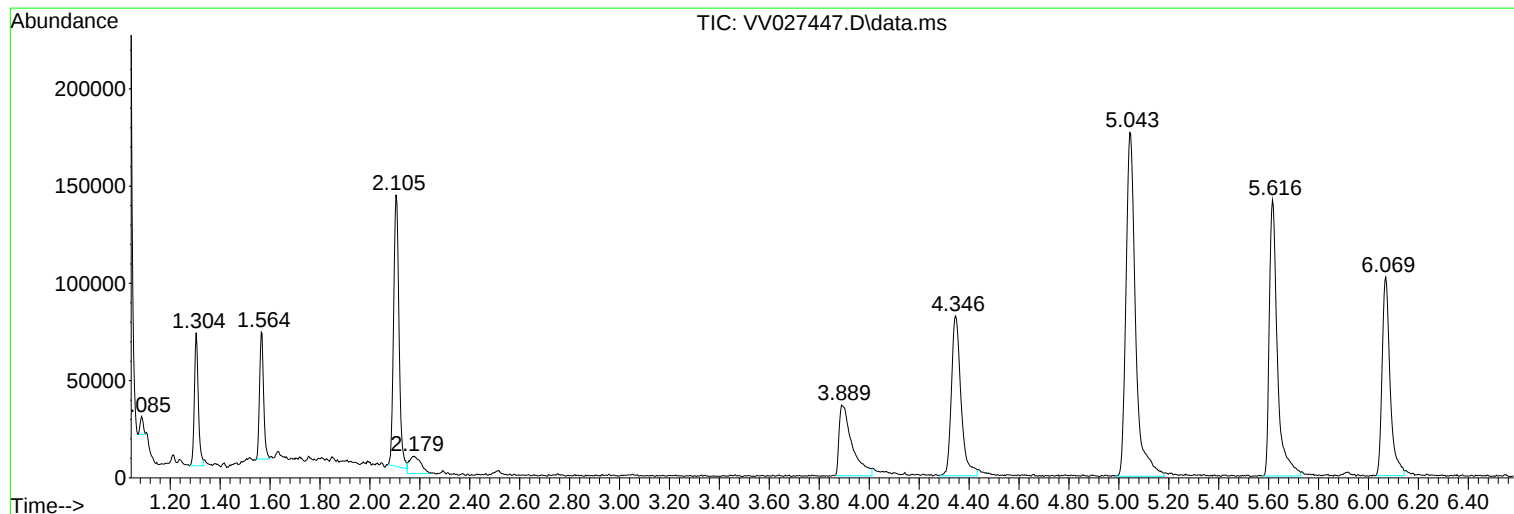

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027447.D
Acq On : 19 Aug 2022 17:58
Operator : SY/MD
Sample : N4253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
Data File : VV027447.D
Acq On : 19 Aug 2022 17:58
Operator : SY/MD
Sample : N4253-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc