
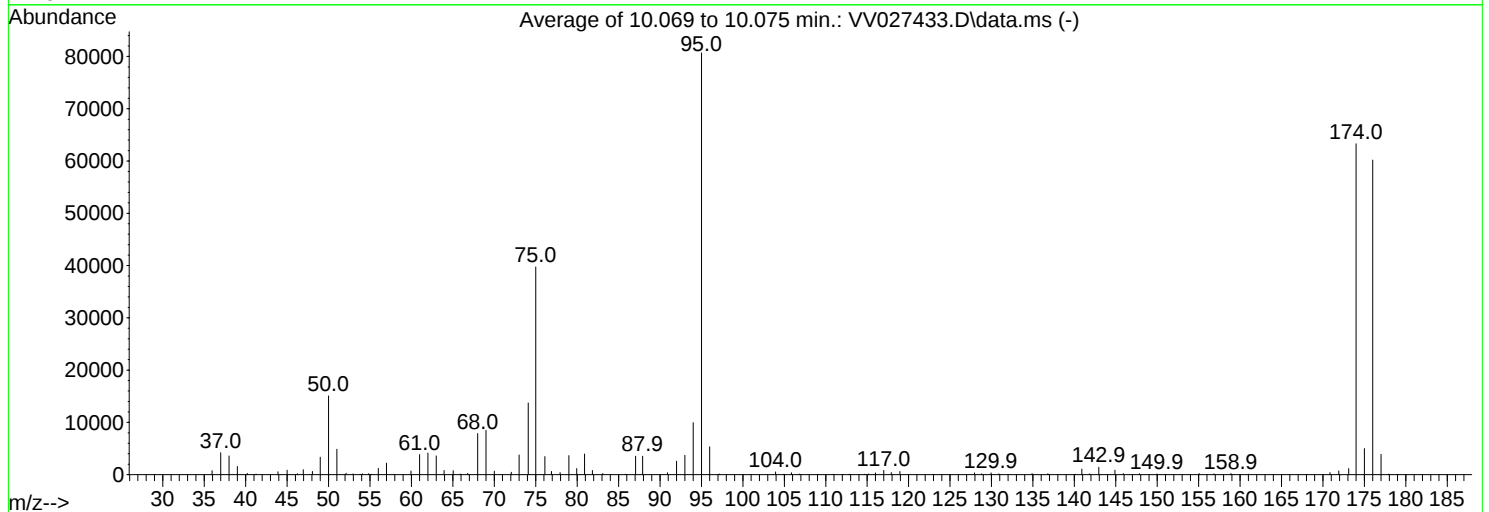


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081922\
 Data File : VV027433.D
 Acq On : 19 Aug 2022 09:22
 Operator : SY/MD
 Sample : BFB356
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB356

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 20 05:55:43 2022

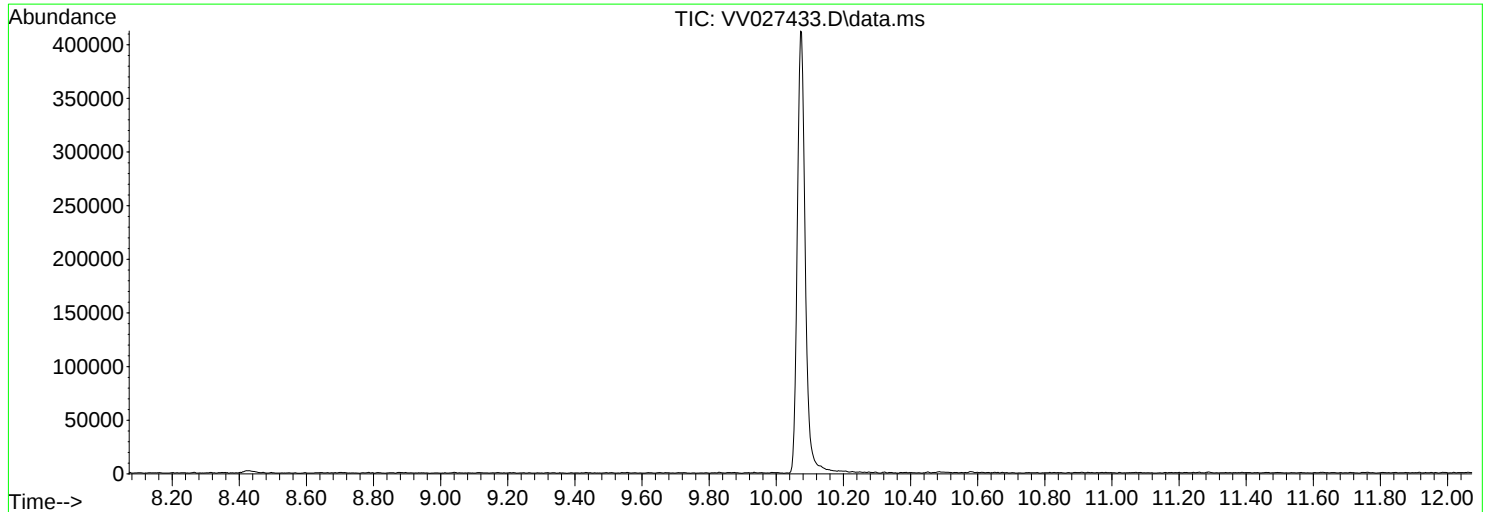

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	15057	PASS
75	95	30	80	49.2	39728	PASS
95	95	100	100	100.0	80693	PASS
96	95	5	9	6.6	5334	PASS
173	174	0.00	2	1.8	1154	PASS
174	95	50	120	78.4	63296	PASS
175	174	5	9	7.9	4980	PASS
176	174	95	105	95.1	60192	PASS
177	176	5	10	6.5	3891	PASS

Scan 2796 (10.030 min): VV027433.D\data.ms
BFB356

m/z	Abundance
36.60	103.0
38.10	144.0
39.90	312.0
43.90	330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
35.90	825.0
37.00	3803.0
38.00	3534.0
39.00	1565.0
41.30	113.0
43.90	890.0
45.00	786.0
46.20	178.0
46.90	921.0
48.00	618.0
49.00	3125.0
50.00	14291.0
51.00	4544.0
52.10	257.0
53.10	139.0
54.10	132.0
55.20	180.0
56.00	1222.0
57.00	2024.0
58.00	103.0
60.00	643.0
61.00	3700.0
62.00	3859.0
63.00	3360.0
63.90	773.0
65.10	630.0
65.90	127.0
66.80	213.0
68.00	7479.0
69.00	8167.0
70.00	620.0
72.00	413.0
73.00	3666.0
74.10	13249.0
75.00	37792.0
76.10	3294.0
76.90	596.0
77.90	401.0
79.00	3512.0
79.90	981.0
80.90	3595.0
81.80	748.0
83.10	187.0
87.00	3346.0
87.90	3265.0
90.90	309.0
92.00	2500.0
93.00	3574.0
94.00	9669.0
95.00	76072.0
96.00	4930.0
97.10	139.0
104.00	435.0
105.00	137.0
105.80	394.0
106.80	108.0
114.60	102.0
115.10	104.0
116.00	322.0
117.00	796.0
117.90	375.0
119.00	577.0
127.90	352.0
128.80	160.0
129.90	327.0
131.00	199.0
134.90	212.0
136.80	132.0
140.90	961.0
141.80	167.0
142.90	1377.0
144.90	924.0
145.90	186.0
147.80	148.0
149.90	133.0
155.10	216.0
156.80	129.0
158.90	246.0
170.80	354.0
171.90	670.0
173.10	1074.0
174.00	58144.0
175.00	4748.0
176.00	54352.0
177.00	3812.0
178.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.00	780.0
37.00	4355.0
38.00	3926.0
39.00	1581.0
40.20	387.0
41.30	130.0
43.90	888.0
45.00	884.0
46.30	199.0
47.00	955.0
48.10	620.0
49.00	3428.0
50.00	15639.0
51.00	5116.0
52.10	292.0
52.90	144.0
54.10	168.0
54.80	244.0
56.00	1241.0
57.00	2301.0
57.90	103.0
59.90	740.0
61.00	3935.0
62.00	4203.0
63.00	3670.0
63.90	833.0
65.00	795.0
65.90	140.0
66.80	252.0
68.00	8085.0
69.00	8723.0
70.00	705.0
72.00	481.0
73.00	3894.0
74.10	14083.0
75.00	40872.0
76.10	3593.0
76.90	637.0
78.00	421.0
79.00	3778.0
79.90	1212.0
80.90	4105.0
81.90	829.0
83.10	226.0
85.80	110.0
87.00	3648.0
87.90	3702.0
90.90	360.0
92.00	2696.0
93.00	3777.0
94.00	10375.0
95.00	83288.0
96.00	5529.0
97.10	121.0
103.90	580.0
104.90	116.0
105.80	383.0
106.80	110.0
110.90	129.0
112.80	117.0
114.70	120.0
115.10	120.0
116.00	352.0
117.00	880.0
117.90	428.0
119.00	652.0
128.00	352.0
128.80	154.0
129.90	356.0
130.90	174.0
134.90	225.0
136.80	188.0
140.10	128.0
140.90	1110.0
141.80	175.0
143.00	1421.0
144.90	918.0
145.90	220.0
147.80	174.0
149.90	139.0
155.10	215.0
156.80	149.0
158.90	208.0
161.00	145.0
170.90	399.0
171.90	723.0
173.10	1207.0
174.00	65328.0
175.00	5153.0
176.00	62176.0
177.00	4063.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.00	725.0
37.00	4385.0
38.00	3741.0
39.00	1567.0
40.20	346.0
41.20	128.0
44.00	833.0
45.00	917.0
46.30	212.0
47.00	949.0
48.10	577.0
49.00	3420.0
50.00	15242.0
51.00	4968.0
52.10	301.0
52.90	161.0
53.80	145.0
54.10	157.0
54.90	313.0
56.00	1159.0
57.00	2342.0
57.80	114.0
60.00	735.0
61.00	3876.0
62.00	4304.0
63.00	3688.0
64.00	769.0
65.00	905.0
65.90	104.0
66.80	252.0
68.00	8043.0
69.00	8534.0
70.00	681.0
72.10	467.0
73.00	3702.0
74.10	13771.0
75.00	40520.0
76.10	3499.0
76.90	568.0
78.00	408.0
79.00	3655.0
80.00	1289.0
80.90	4150.0
81.90	858.0
83.10	192.0
85.80	130.0
86.00	129.0
87.10	3556.0
87.90	3643.0
90.90	418.0
92.00	2519.0
93.00	3761.0
94.00	9837.0
95.00	82720.0
96.00	5544.0
97.20	108.0
103.90	591.0
105.90	354.0
106.80	122.0
110.90	129.0
112.10	108.0
112.80	128.0
114.70	101.0
115.20	121.0
116.00	361.0
117.00	785.0
117.90	430.0
118.90	658.0
128.00	299.0
128.80	134.0
130.00	354.0
130.80	140.0
134.90	193.0
136.80	235.0
140.10	139.0
140.90	1108.0
141.90	130.0
142.90	1482.0
144.90	769.0
145.90	198.0
147.90	210.0
150.00	142.0
154.90	178.0
156.90	174.0
158.90	168.0
161.00	139.0
170.90	427.0
171.90	745.0
173.10	1182.0
174.00	66416.0
175.00	5040.0
176.00	64048.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

177.00	3797.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356