
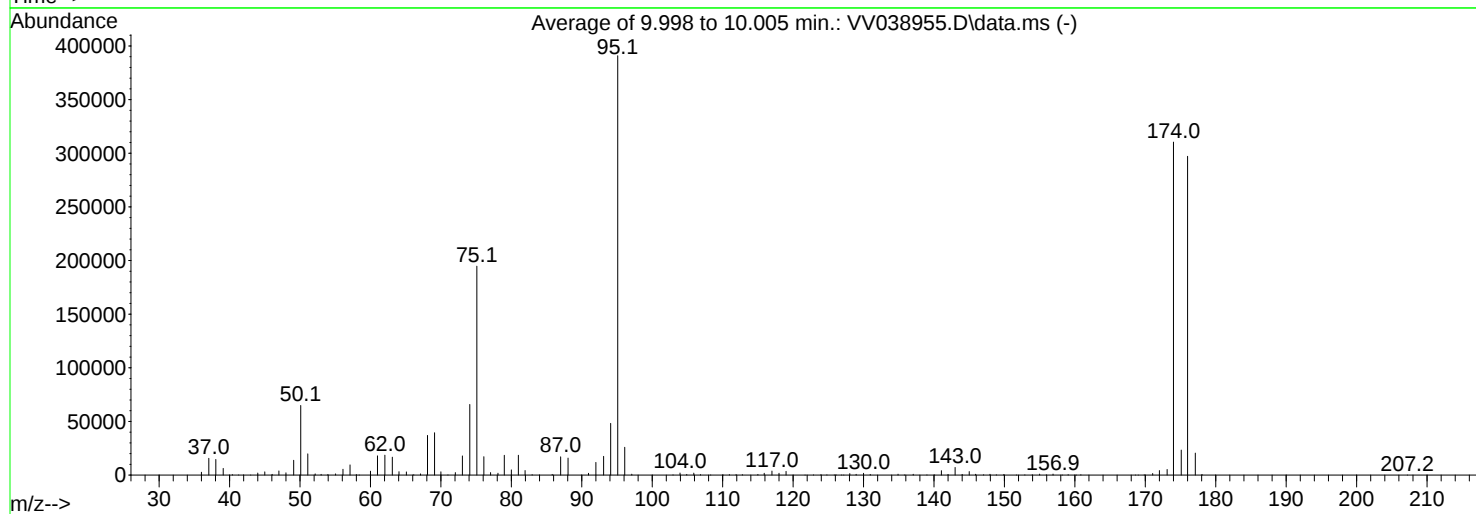


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV081925\
Data File : VV038955.D
Acq On : 19 Aug 2025 09:52
Operator : SY/MD
Sample : BFB239
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB239

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM081925.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 20 03:16:00 2025

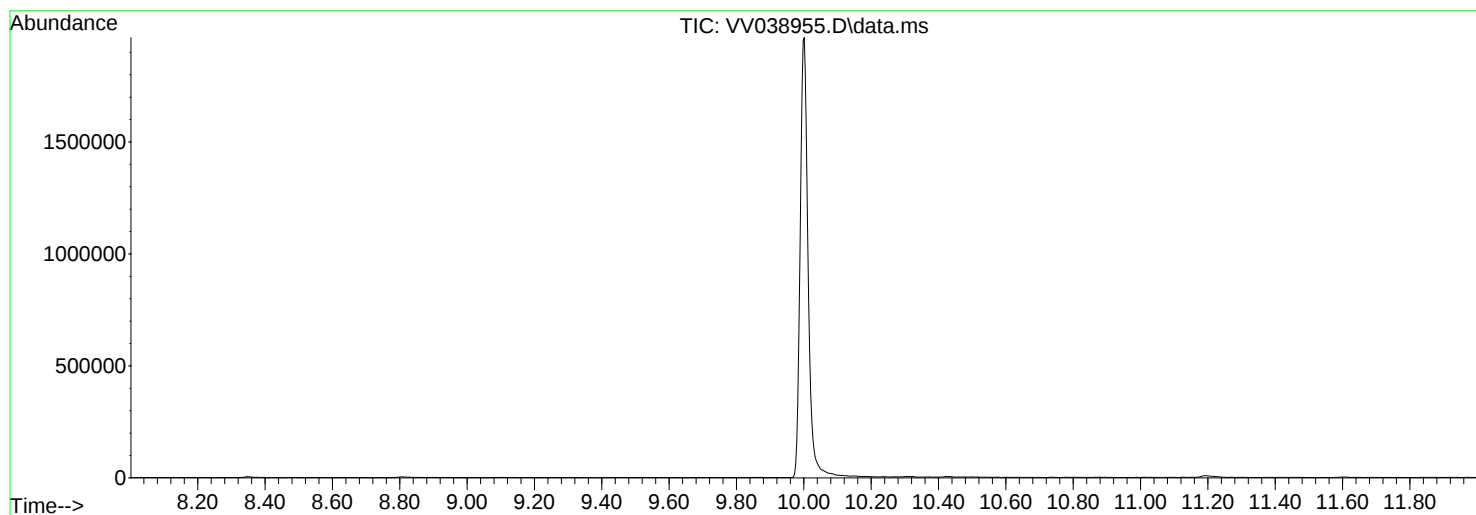

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2773

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	64883	PASS
75	95	30	80	49.8	194752	PASS
95	95	100	100	100.0	390912	PASS
96	95	5	9	6.6	25888	PASS
173	174	0.00	2	1.7	5252	PASS
174	95	50	120	79.4	310400	PASS
175	174	5	9	7.5	23333	PASS
176	174	95	101	95.7	297173	PASS
177	176	5	9	6.9	20493	PASS