

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082018\
 Data File : VV007067.D
 Acq On : 20 Aug 2018 12:24
 Operator : SY/MD
 Sample : VV0820WBL01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK63

Quant Time: Aug 21 04:17:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 21 04:05:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	259150	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	251945	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	98865	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	83185	4.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.40%
7) Chloroethane-d5	1.58	69	79399	5.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.00%
11) 1,1-Dichloroethene-d2	2.13	63	121287	3.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.20%
20) 2-Butanone-d5	3.97	46	222499	46.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.50%
24) Chloroform-d	4.40	84	187071	5.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.20%
26) 1,2-Dichloroethane-d4	5.09	65	93324	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.00%
32) Benzene-d6	5.10	84	365383	5.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	113.00%
36) 1,2-Dichloropropane-d6	6.12	67	121805	5.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.20%
41) Toluene-d8	7.36	98	276288	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
43) trans-1,3-Dichloropropene-	7.67	79	37562	4.88	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.60%
46) 2-Hexanone-d5	8.15	63	106845	33.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	87616	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	98191	5.71	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.20%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	10589	0.47 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082018\
Data File : VV007067.D
Acq On : 20 Aug 2018 12:24
Operator : SY/MD
Sample : VV0820WBL01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK63

Quant Time: Aug 21 04:17:14 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 04:05:27 2018
Response via : Initial Calibration

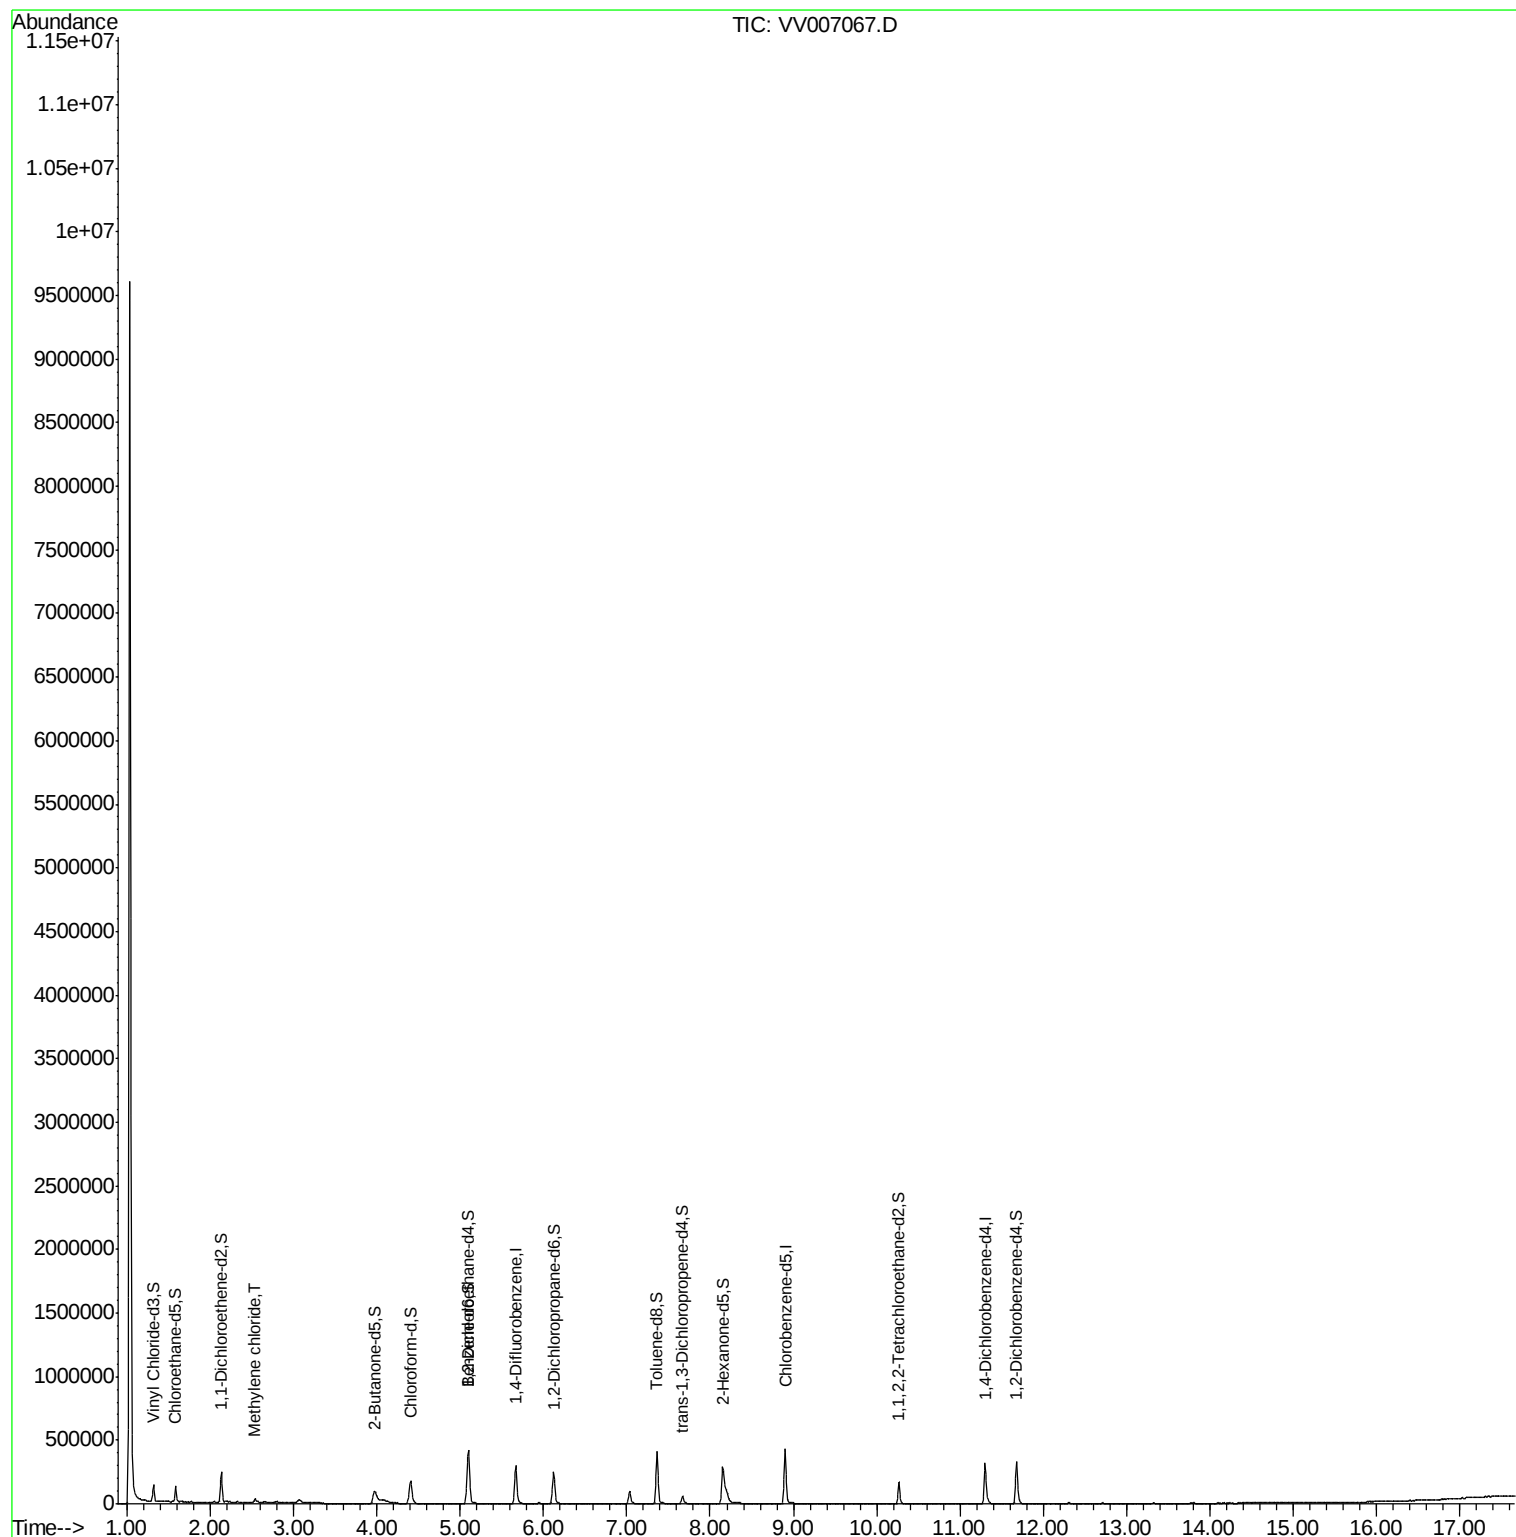

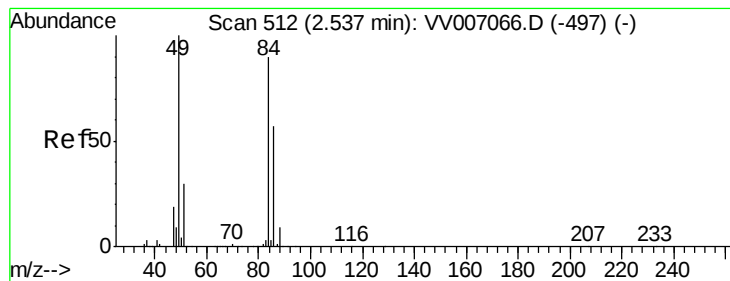

#16

Methylene chloride

Concen: 0.47 ug/L

RT: 2.54 min Scan# 512

Delta R.T. -0.00 min

Lab File: VV007067.D

Acq: 20 Aug 2018 12:24

Instrument :

MSVOA_V

ClientSampleId :

VBLK63

Tot Ion: 84 Resp: 10589

Ion Ratio Lower Upper

84 100

86 67.5 45.7 84.9

49 105.0 78.8 146.4

