

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082018\
 Data File : VV007090.D
 Acq On : 20 Aug 2018 23:33
 Operator : SY/MD
 Sample : J4515-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0324

Quant Time: Aug 21 07:05:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 21 05:25:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	237221	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	240870	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	89872	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	77719	5.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.60%
7) Chloroethane-d5	1.58	69	70446	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.40%
11) 1,1-Dichloroethene-d2	2.13	63	112216	3.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.00%
20) 2-Butanone-d5	3.97	46	229724	52.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.34%
24) Chloroform-d	4.41	84	170002	5.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.40%
26) 1,2-Dichloroethane-d4	5.09	65	87994	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.20%
32) Benzene-d6	5.10	84	316233	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	6.12	67	110949	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	7.37	98	231176	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.67	79	21422	2.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.20%
46) 2-Hexanone-d5	8.15	63	77666	25.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	51.62%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	83151	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	84612	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	6001	2.65 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082018\
Data File : VV007090.D
Acq On : 20 Aug 2018 23:33
Operator : SY/MD
Sample : J4515-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0324

Quant Time: Aug 21 07:05:36 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 05:25:12 2018
Response via : Initial Calibration

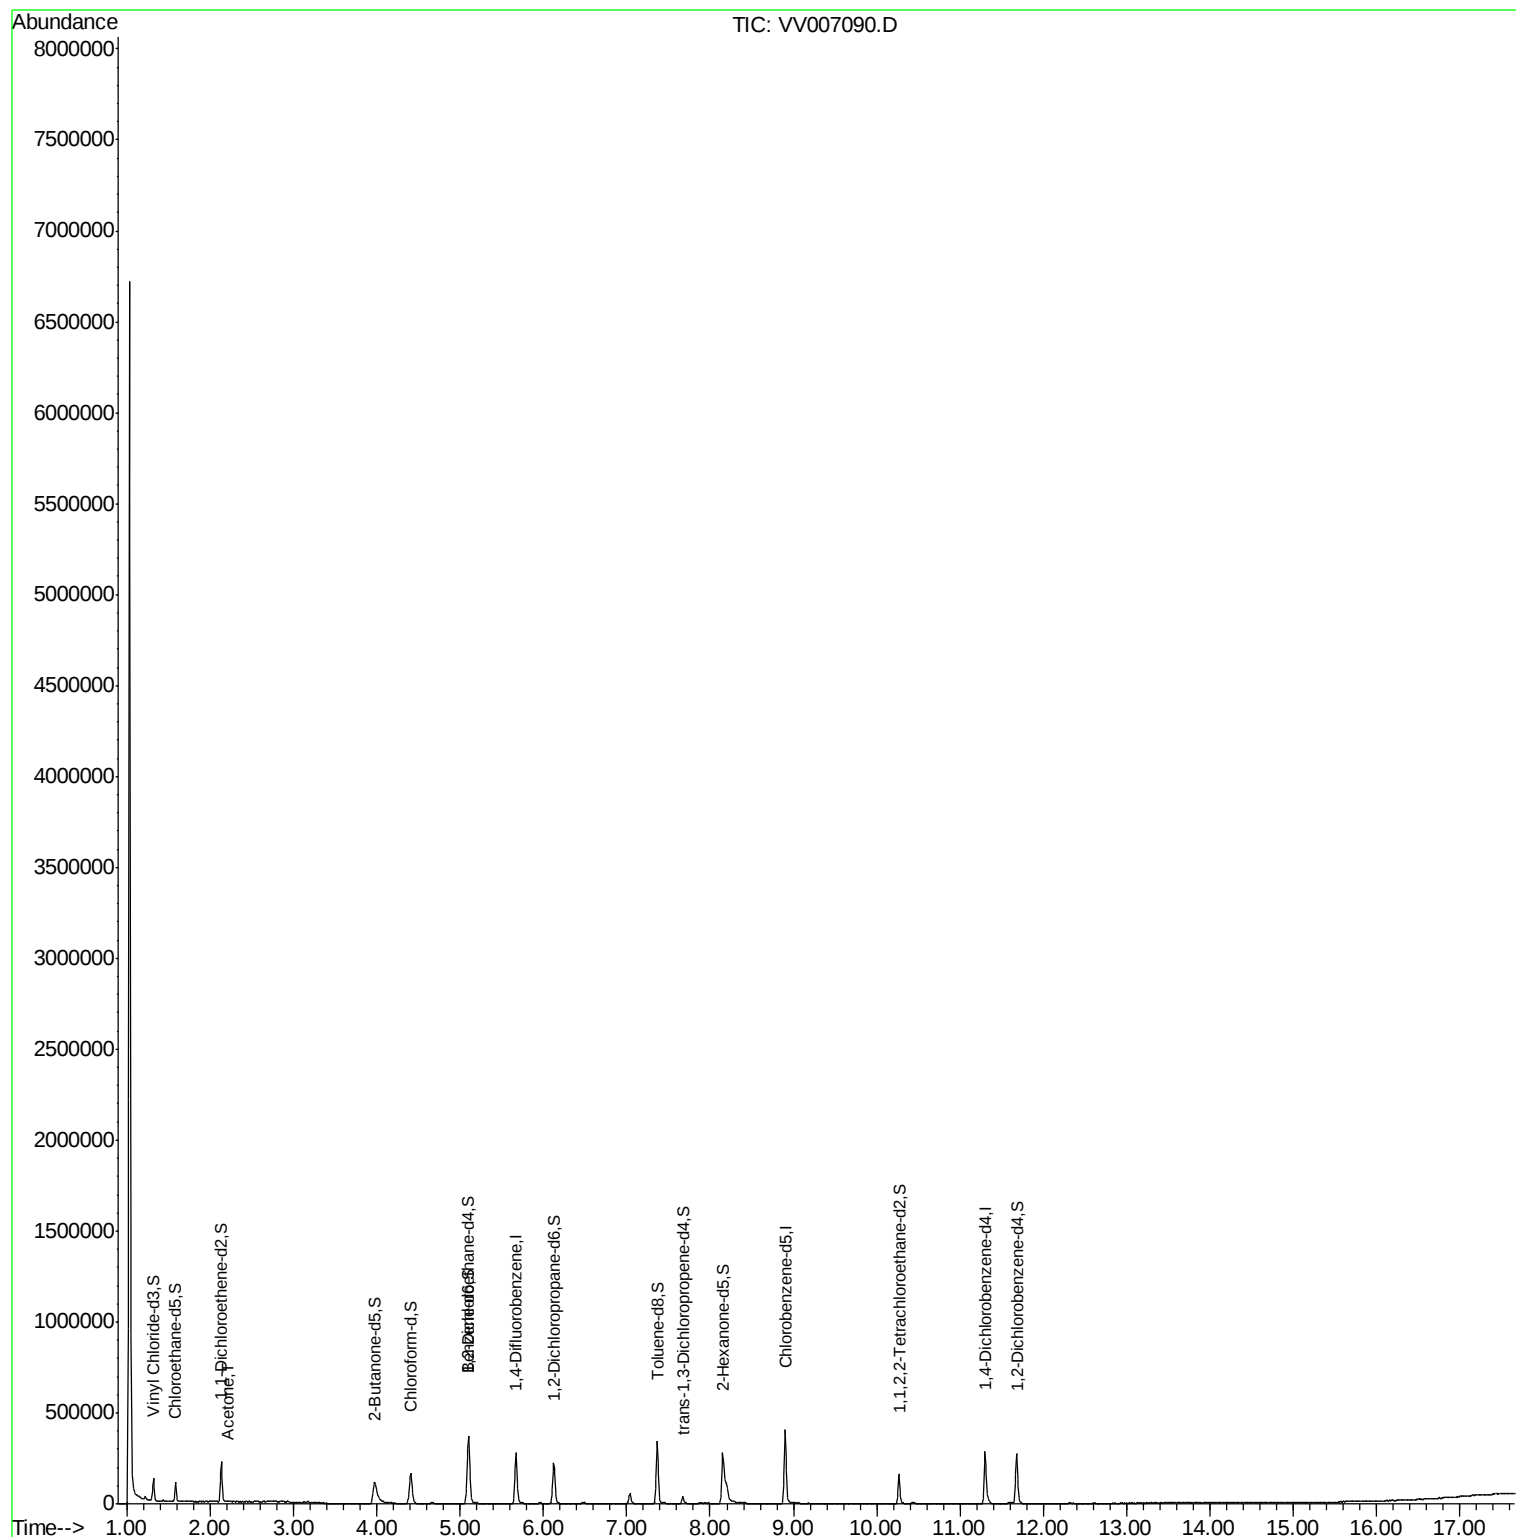

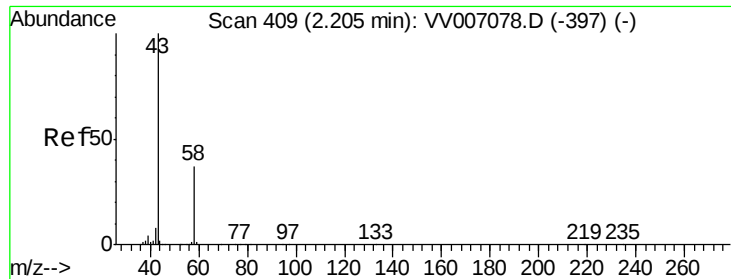

#13

Acetone

Concen: 2.65 ug/L

RT: 2.21 min Scan# 412

Delta R.T. 0.01 min

Lab File: VV007090.D

Acq: 20 Aug 2018 23:33

Instrument :

MSVOA_V

ClientSampleId :

C0324

Tot Ion: 43 Resp: 6001

Ion Ratio Lower Upper

43 100

58 36.9 0.0 71.4

