

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082018\
 Data File : VV007094.D
 Acq On : 21 Aug 2018 01:19
 Operator : SY/MD
 Sample : J4515-07
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0344

Quant Time: Aug 21 09:22:03 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 21 05:25:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	238994	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	239510	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	89980	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	76491	4.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.20%
7) Chloroethane-d5	1.58	69	70462	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.60%
11) 1,1-Dichloroethene-d2	2.13	63	111500	3.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.00%
20) 2-Butanone-d5	3.97	46	230173	51.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.76%
24) Chloroform-d	4.40	84	167174	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	5.09	65	90178	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.20%
32) Benzene-d6	5.10	84	317328	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
36) 1,2-Dichloropropane-d6	6.12	67	109703	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.37	98	229584	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.67	79	20445	2.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	55.80%
46) 2-Hexanone-d5	8.15	63	82261	27.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	54.98%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	83978	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	81871	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	4413	1.93 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082018\
Data File : VV007094.D
Acq On : 21 Aug 2018 01:19
Operator : SY/MD
Sample : J4515-07
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0344

Quant Time: Aug 21 09:22:03 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR080918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 21 05:25:12 2018
Response via : Initial Calibration

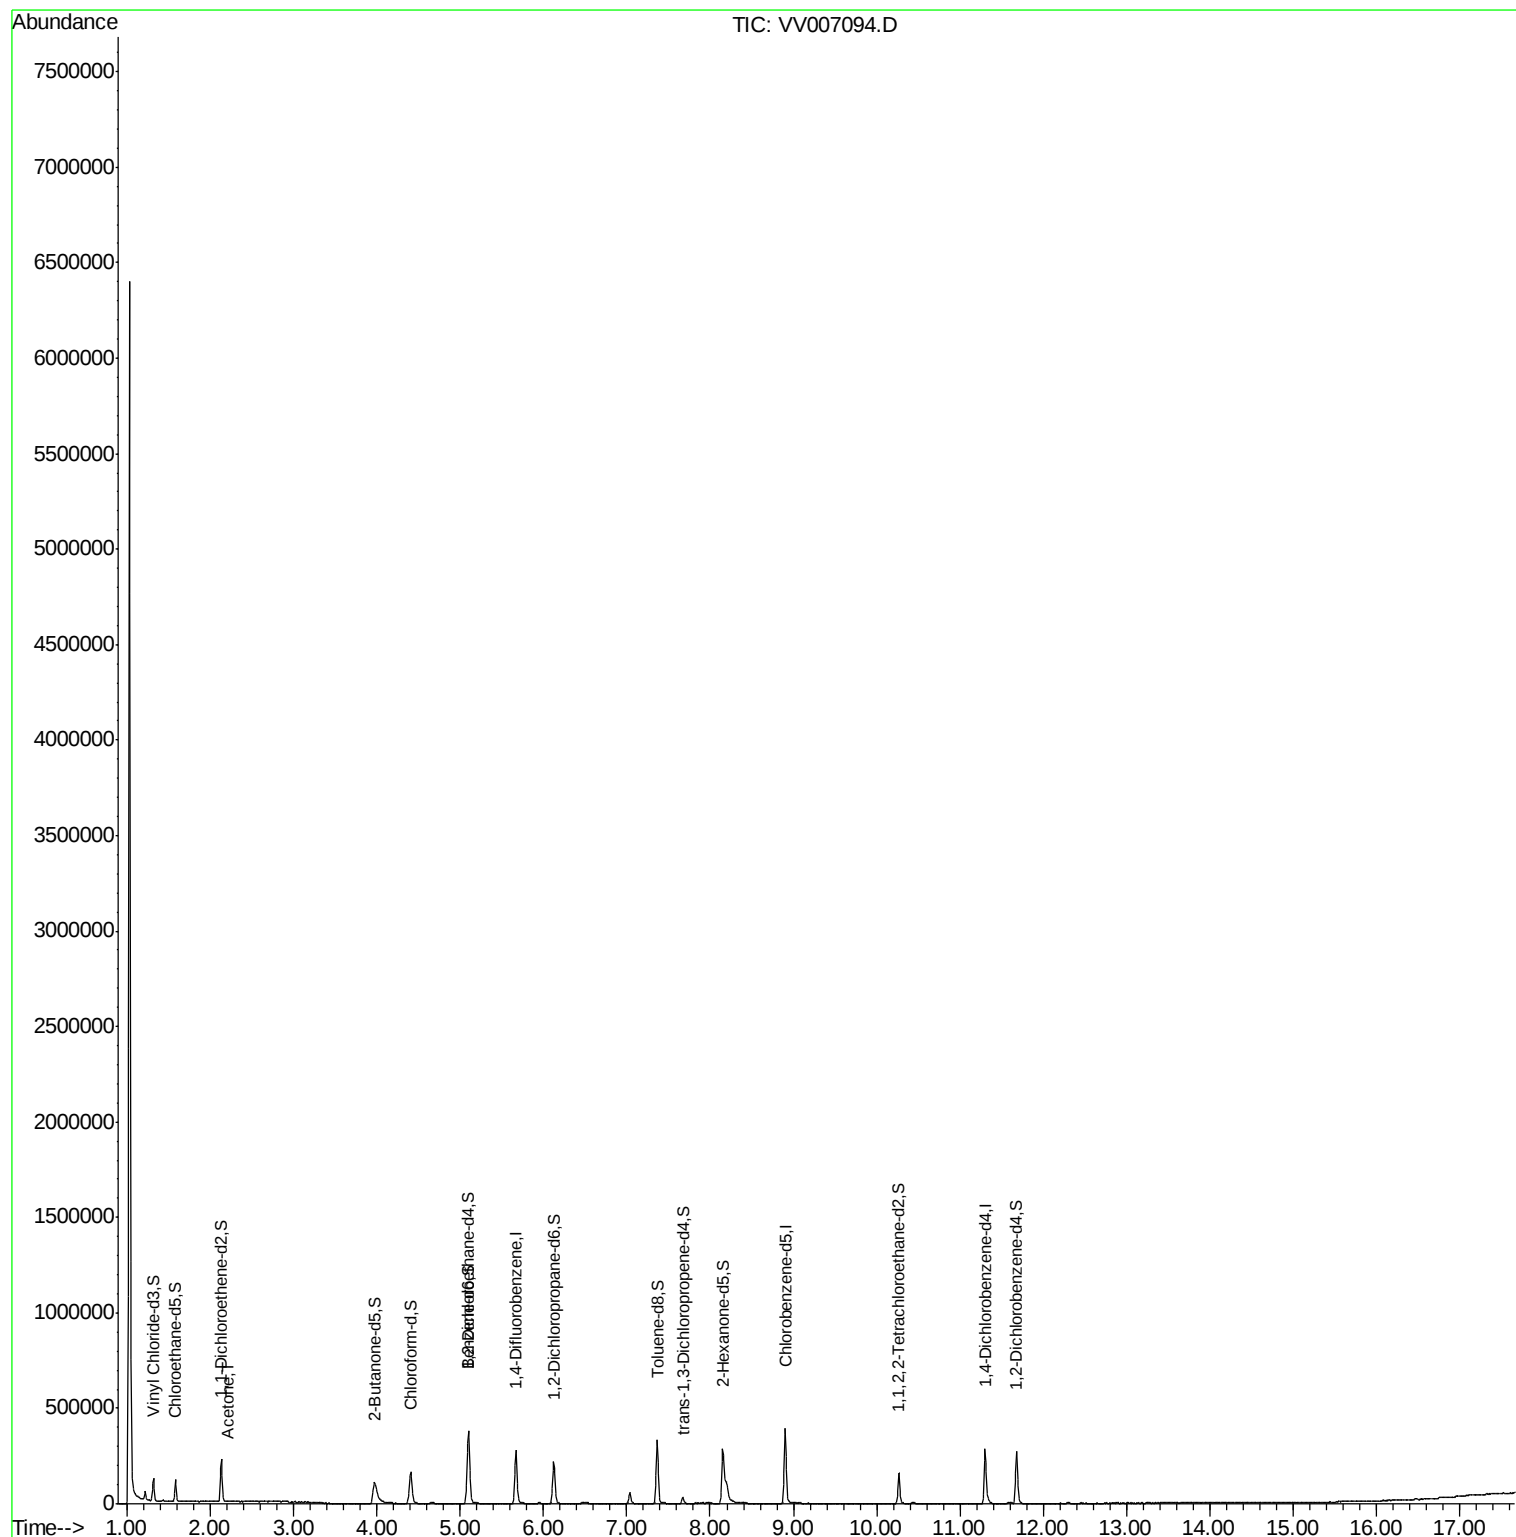

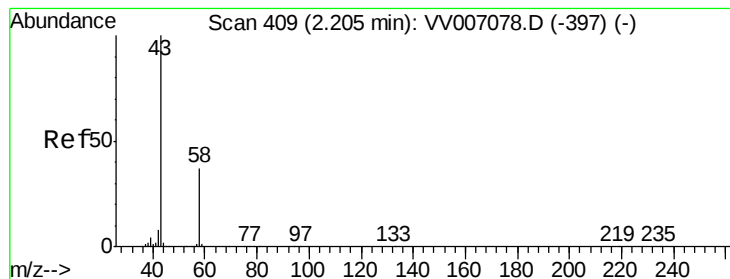

#13

Acetone

Concen: 1.93 ug/L

RT: 2.21 min Scan# 410

Delta R.T. 0.00 min

Lab File: VV007094.D

Acq: 21 Aug 2018 01:19

Instrument :
MSVOA_V
ClientSampleId :
C0344

Tot Ion: 43 Resp: 4413

Ion Ratio Lower Upper

43 100

58 43.7 0.0 71.4

