


Data File : VV012307.D
Acq On : 20 Aug 2019 12:34
Operator : SY/MD
Sample : K4395-04DL 4X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 21 02:01:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 21 01:13:54 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0AE2DL

Manual Integrations
APPROVED

MMDadoda
8/22/2019 8:28:04 AM

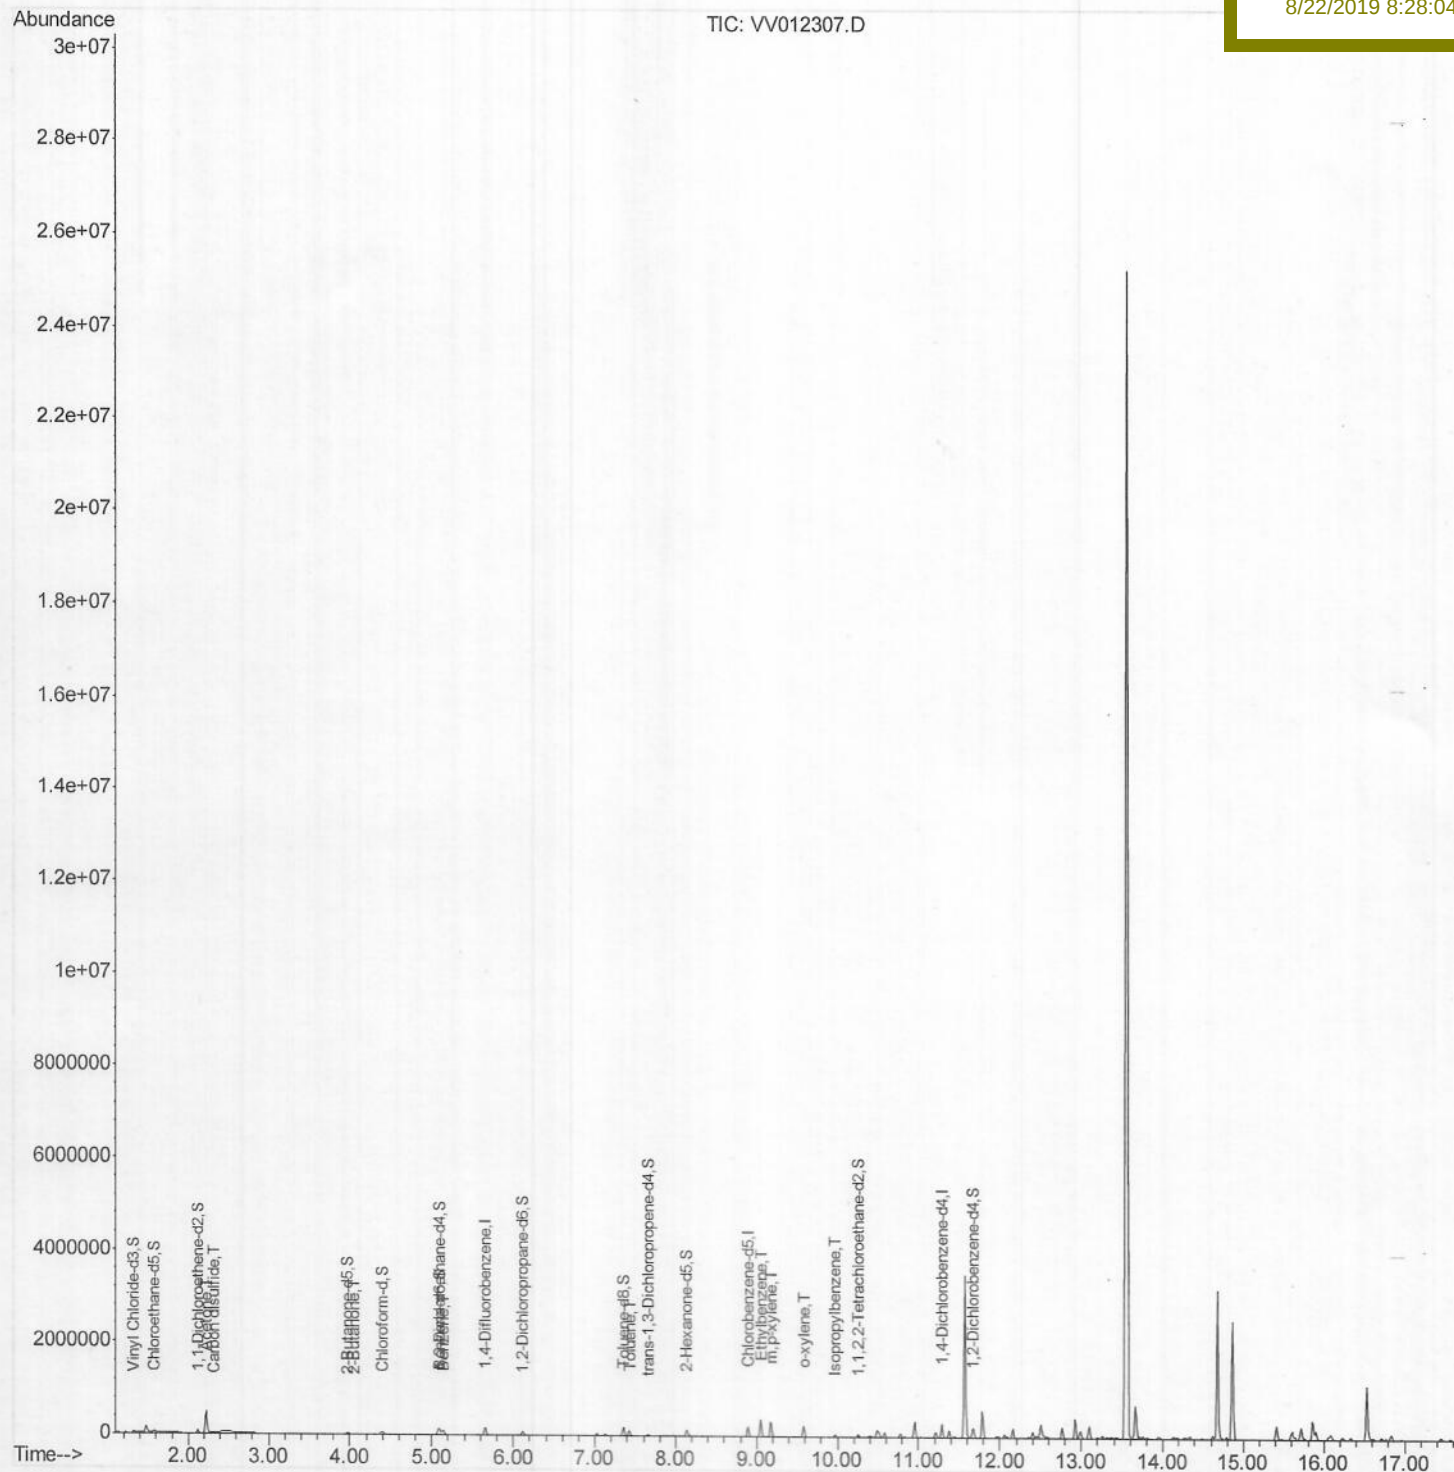

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082019\
Quantitation Report (Qedit)




Data File : VV012307.D
Acq On : 20 Aug 2019 12:34
Operator : SY/MD
Sample : K4395-04DL 4X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 21 01:54:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 21 01:13:54 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0AE2DL

Manual Integrations
APPROVED

MMDadoda
8/22/2019 8:28:04 AM

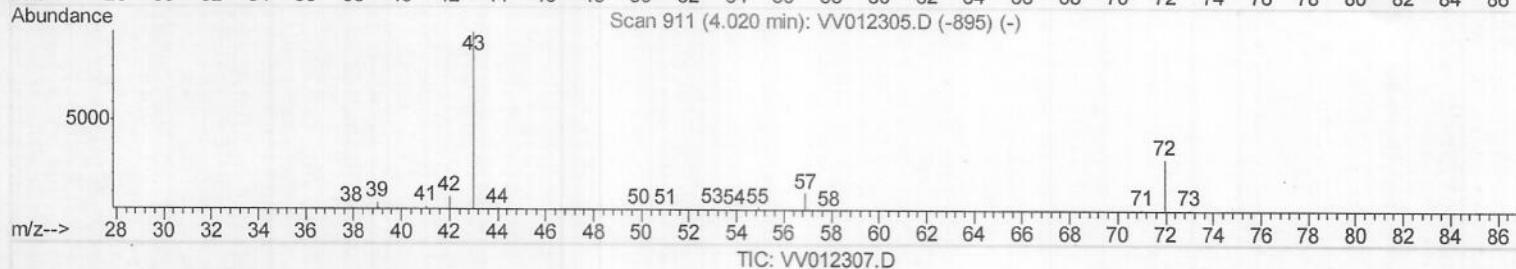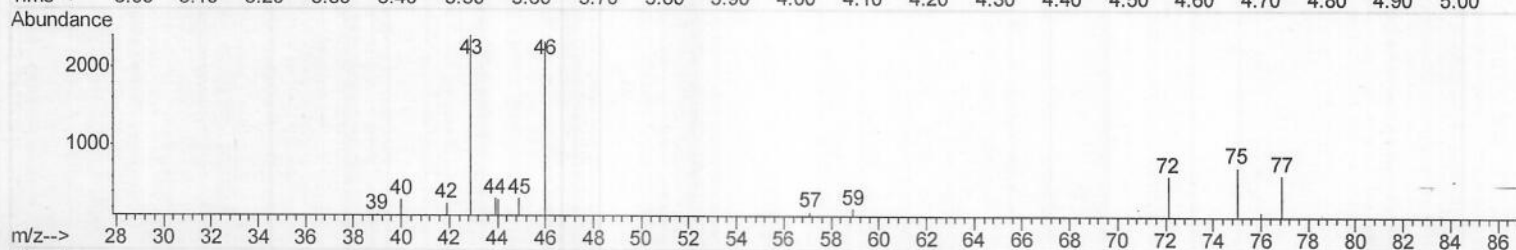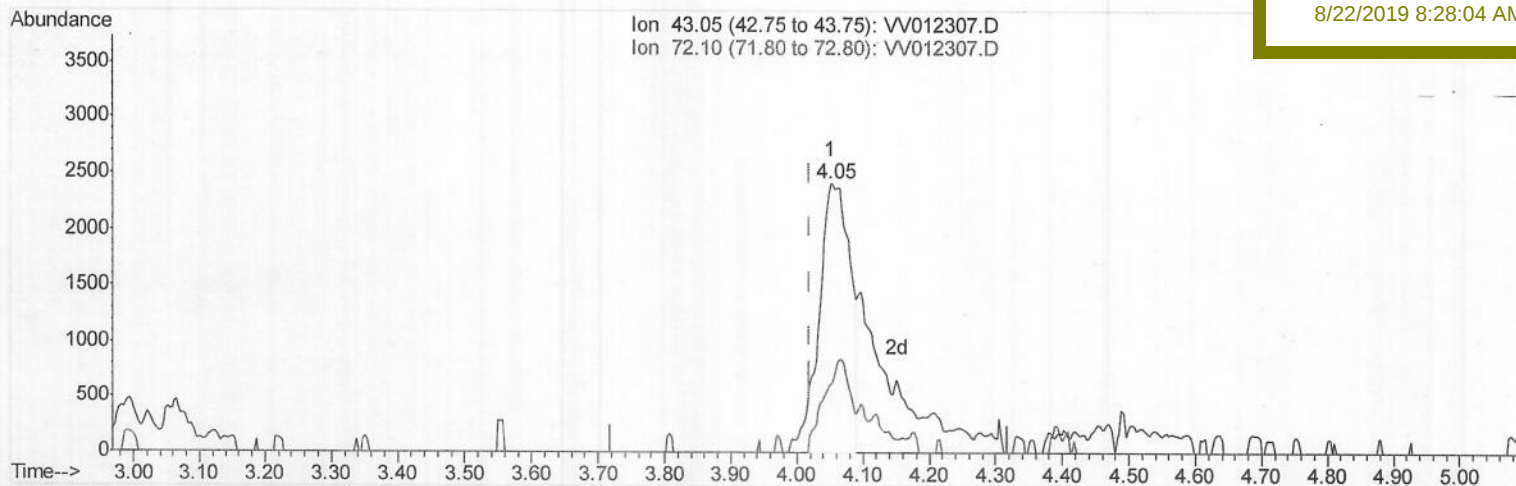

(21) 2-Butanone (T)

4.052min (+0.032) 4.34ug/L

response 7966

Ion	Exp%	Act%
43.05	100	100
72.10	29.60	29.29
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VV012307.D
Acq On : 20 Aug 2019 12:34
Operator : SY/MD
Sample : K4395-04DL 4X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 21 01:54:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 21 01:13:54 2019
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
C0AE2DL

Manual Integrations
APPROVED

MMDadoda
8/22/2019 8:28:04 AM

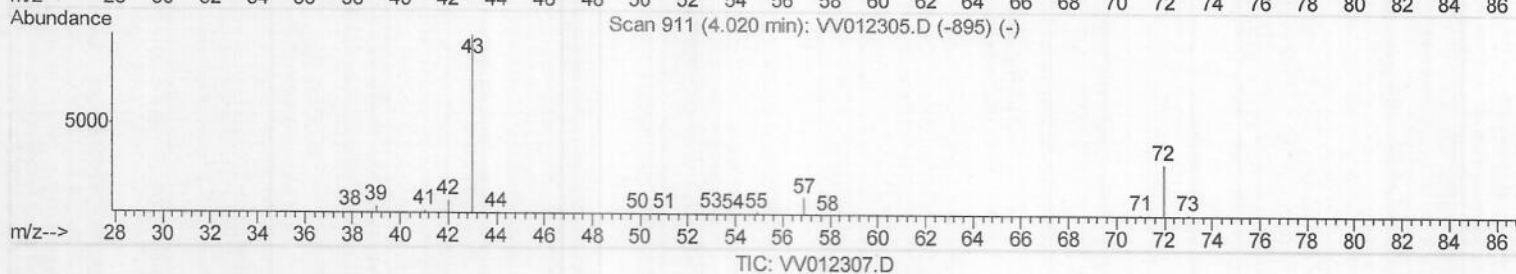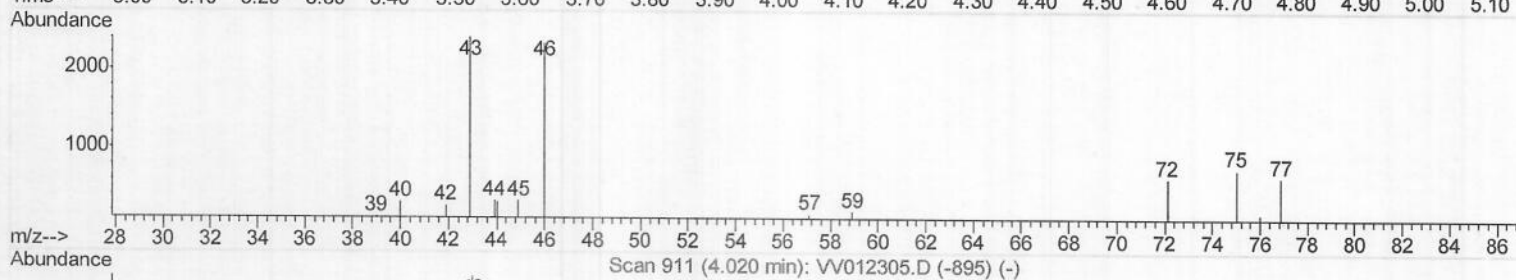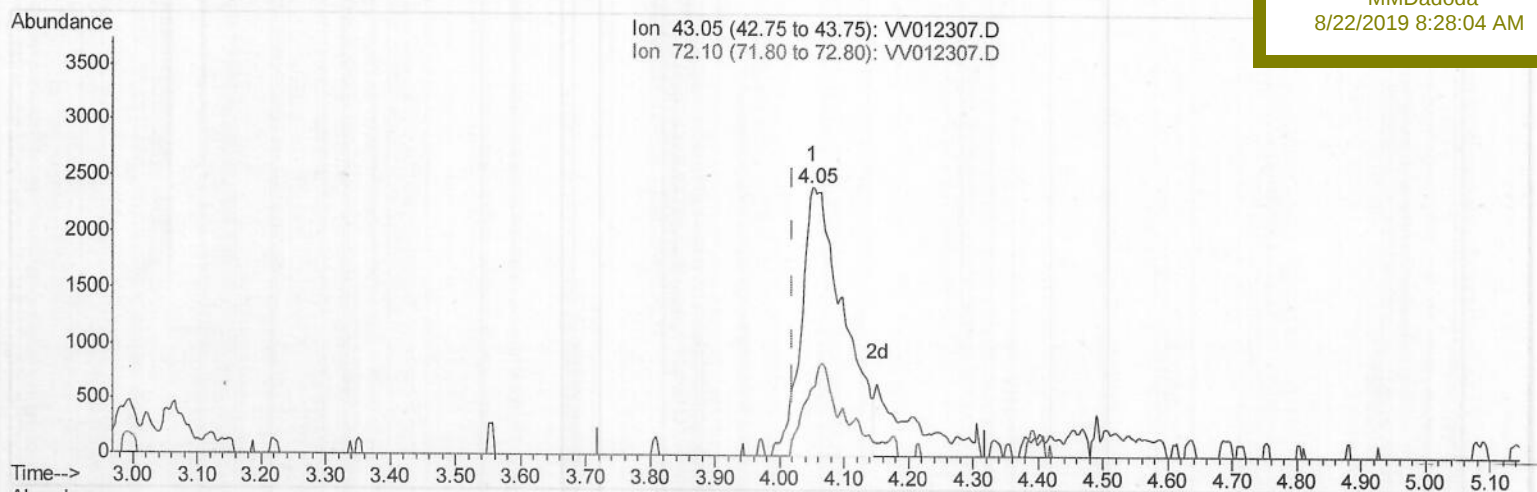

(21) 2-Butanone (T)

4.052min (+0.032) 6.04ug/L m) M009/28/19

response 11080

Ion	Exp%	Act%
43.05	100	100
72.10	29.60	21.06
0.00	0.00	0.00
0.00	0.00	0.00

Data File : VV012307.D

Acq On : 20 Aug 2019 12:34

Operator : SY/MD

Sample : K4395-04DL 4X

Misc : 25mL/MSVOA_V/WATER

ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 21 02:01:00 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Wed Aug 21 01:13:54 2019

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :

C0AE2DL

Manual Integrations

APPROVED

MMDadoda

8/22/2019 8:28:04 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	134191	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	124169	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	71036	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	18233	2.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	53.20%
7) Chloroethane-d5	1.58	69	15141	3.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	60.40%#
11) 1,1-Dichloroethene-d2	2.13	63	30892	2.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	47.40%#
20) 2-Butanone-d5	3.97	46	48494	26.23	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	52.46%
24) Chloroform-d	4.39	84	63008	3.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	68.00%#
26) 1,2-Dichloroethane-d4	5.08	65	31233	3.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	65.40%#
32) Benzene-d6	5.09	84	120585	3.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.40%
36) 1,2-Dichloropropane-d6	6.11	67	31932	3.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	68.80%
41) Toluene-d8	7.36	98	117510	3.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.80%
43) trans-1,3-Dichloropropene-	7.66	79	14219	3.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.20%
46) 2-Hexanone-d5	8.14	63	52215	41.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.96%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	23872	3.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	67.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	51899	3.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	72.60%#

Target Compounds

					Qvalue	
13) Acetone	2.23	43	57380	59.338	ug/L	# 29
14) Carbon disulfide	2.31	76	16773	0.981	ug/L	97
21) 2-Butanone	4.05	43	11080m)	6.039	ug/L	100
33) Benzene	5.14	78	88374	2.573	ug/L	95
42) Toluene	7.43	91	83661	2.201	ug/L	95
52) Ethylbenzene	9.05	91	256476	6.030	ug/L	99
53) m,p-xylene	9.18	106	89215	5.373	ug/L	97
54) o-xylene	9.58	106	61065	3.824	ug/L	90
56) Isopropylbenzene	9.97	105	36431	0.826	ug/L	98

(#)=qualifier out of range (m)=manual integration (+)=signals summed

JMD08/28/19