


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082019\
Data File : VV012304.D
Acq On : 20 Aug 2019 08:39
Operator : SY/MD
Sample : BFB51
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB51

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR081919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Aug 22 16:11:35 2019

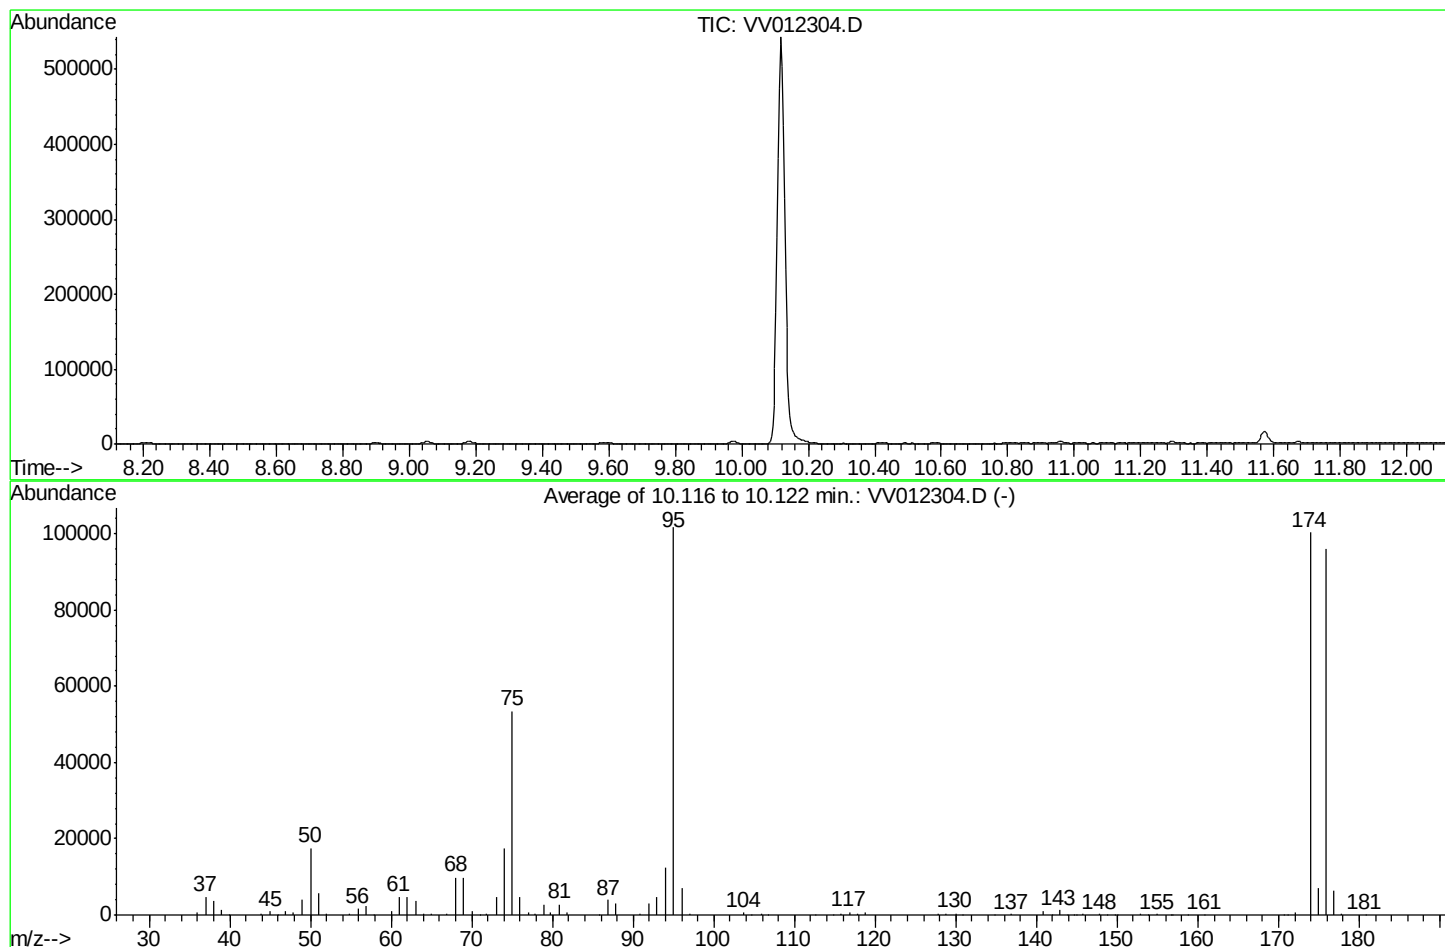

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	17541	PASS
75	95	30	80	52.6	53498	PASS
95	95	100	100	100.0	101696	PASS
96	95	5	9	7.0	7069	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.7	100394	PASS
175	174	5	9	7.0	6992	PASS
176	174	95	101	95.7	96042	PASS
177	176	5	9	6.5	6288	PASS

m/z	Abundance
36.00	629.0
37.00	5004.0
38.00	3869.0
38.90	1495.0
40.00	345.0
43.90	703.0
45.00	862.0
45.90	117.0
46.90	995.0
47.80	619.0
49.00	4217.0
50.00	17992.0
51.00	5948.0
51.90	255.0
54.90	239.0
55.90	1635.0
57.00	2523.0
57.80	113.0
60.10	868.0
61.00	5250.0
62.00	4860.0
63.00	3597.0
64.00	411.0
65.00	321.0
66.90	372.0
68.00	10081.0
69.00	9861.0
70.00	823.0
71.00	128.0
71.90	463.0
73.00	4746.0
74.00	17560.0
75.00	54352.0
76.00	4800.0
77.00	720.0
77.70	343.0
78.90	2883.0
79.80	778.0
80.90	2935.0
81.90	688.0
85.70	209.0
87.00	4015.0
87.90	3009.0
90.80	416.0
91.90	3371.0
93.00	4702.0
94.00	12744.0
95.00	103752.0
96.00	7325.0
97.00	267.0
103.80	531.0
104.70	155.0
105.90	397.0
114.80	163.0
115.80	443.0
116.80	888.0
117.80	457.0
118.80	549.0
127.90	338.0
128.80	274.0
129.90	556.0
130.90	136.0
134.90	144.0
136.90	283.0
140.80	1147.0
142.00	131.0
142.90	1261.0
143.90	148.0
144.70	117.0
145.70	286.0
147.80	281.0
148.70	105.0
149.70	163.0
152.90	228.0
155.00	275.0
156.70	191.0
158.70	118.0
160.90	154.0
170.70	110.0
171.90	575.0
173.90	99536.0
175.00	7185.0
175.90	95728.0
176.90	6135.0
177.80	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
36.00	603.0
37.00	4915.0
38.00	3644.0
38.90	1470.0
39.90	347.0
43.90	728.0
45.00	905.0
45.90	147.0
46.90	1100.0
47.80	642.0
49.00	4004.0
50.00	18120.0
51.00	5902.0
51.90	312.0
54.80	189.0
55.90	1612.0
57.00	2436.0
57.80	124.0
60.00	972.0
61.00	5005.0
62.00	4627.0
63.00	3746.0
64.00	394.0
64.90	325.0
66.90	360.0
68.00	10132.0
69.00	9962.0
70.00	918.0
71.90	489.0
73.00	4865.0
74.00	18128.0
75.00	55240.0
76.00	4648.0
77.10	626.0
77.70	324.0
78.90	2754.0
79.80	787.0
80.90	2934.0
81.90	642.0
85.70	160.0
86.90	4139.0
87.90	3179.0
90.80	413.0
91.90	3244.0
93.00	4744.0
94.00	12905.0
95.00	104824.0
96.00	7381.0
97.00	298.0
103.80	536.0
104.70	162.0
105.80	407.0
106.70	121.0
112.70	106.0
114.80	164.0
115.80	370.0
116.80	857.0
117.90	448.0
118.80	597.0
127.90	370.0
128.80	310.0
129.90	509.0
130.80	175.0
134.70	174.0
136.90	299.0
140.90	1137.0
141.80	155.0
142.80	1314.0
143.90	123.0
144.70	107.0
145.70	284.0
147.80	254.0
148.70	108.0
150.00	164.0
152.90	214.0
154.90	327.0
156.90	155.0
158.70	105.0
160.90	154.0
172.00	554.0
173.90	103584.0
174.90	7057.0
175.90	99016.0
176.90	6503.0
177.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.90	591.0
37.00	4256.0
38.00	3328.0
38.90	1331.0
39.90	404.0
43.90	659.0
45.00	799.0
45.90	121.0
46.90	1031.0
47.80	535.0
49.00	3479.0
50.00	16512.0
51.00	5193.0
51.90	312.0
54.70	197.0
55.90	1378.0
56.90	2170.0
60.00	997.0
61.00	4269.0
62.00	4240.0
63.00	3563.0
64.10	347.0
65.00	250.0
67.00	290.0
68.00	9415.0
69.00	9113.0
70.00	860.0
71.80	505.0
73.00	4413.0
74.00	16840.0
75.00	50904.0
76.00	4295.0
77.10	488.0
77.80	367.0
78.90	2405.0
79.80	674.0
80.90	2667.0
81.80	539.0
86.90	3846.0
87.90	3047.0
90.90	367.0
91.90	2803.0
92.90	4557.0
94.00	11920.0
95.00	96512.0
96.00	6501.0
97.00	246.0
103.70	513.0
104.70	165.0
105.80	394.0
106.70	104.0
112.60	107.0
114.90	158.0
115.90	265.0
116.80	739.0
117.90	426.0
118.80	619.0
127.80	340.0
128.80	255.0
130.00	385.0
130.90	197.0
134.70	198.0
136.90	247.0
140.90	1031.0
141.90	171.0
142.80	1200.0
145.00	123.0
145.70	235.0
147.90	221.0
150.00	159.0
152.90	178.0
153.80	101.0
154.90	335.0
156.90	155.0
158.80	118.0
160.80	145.0
171.10	136.0
172.10	508.0
173.90	98064.0
174.90	6735.0
175.90	93384.0
176.90	6226.0
177.90	234.0
180.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

Scan 2793 (10.071 min): VV012304.D
BFB51

m/z	Abundance
40.00	269.0
43.80	199.0
44.10	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51