


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082020\
 Data File : VV018064.D
 Acq On : 20 Aug 2020 10:20
 Operator : SY/MD
 Sample : BFB78
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 21 05:53:05 2020

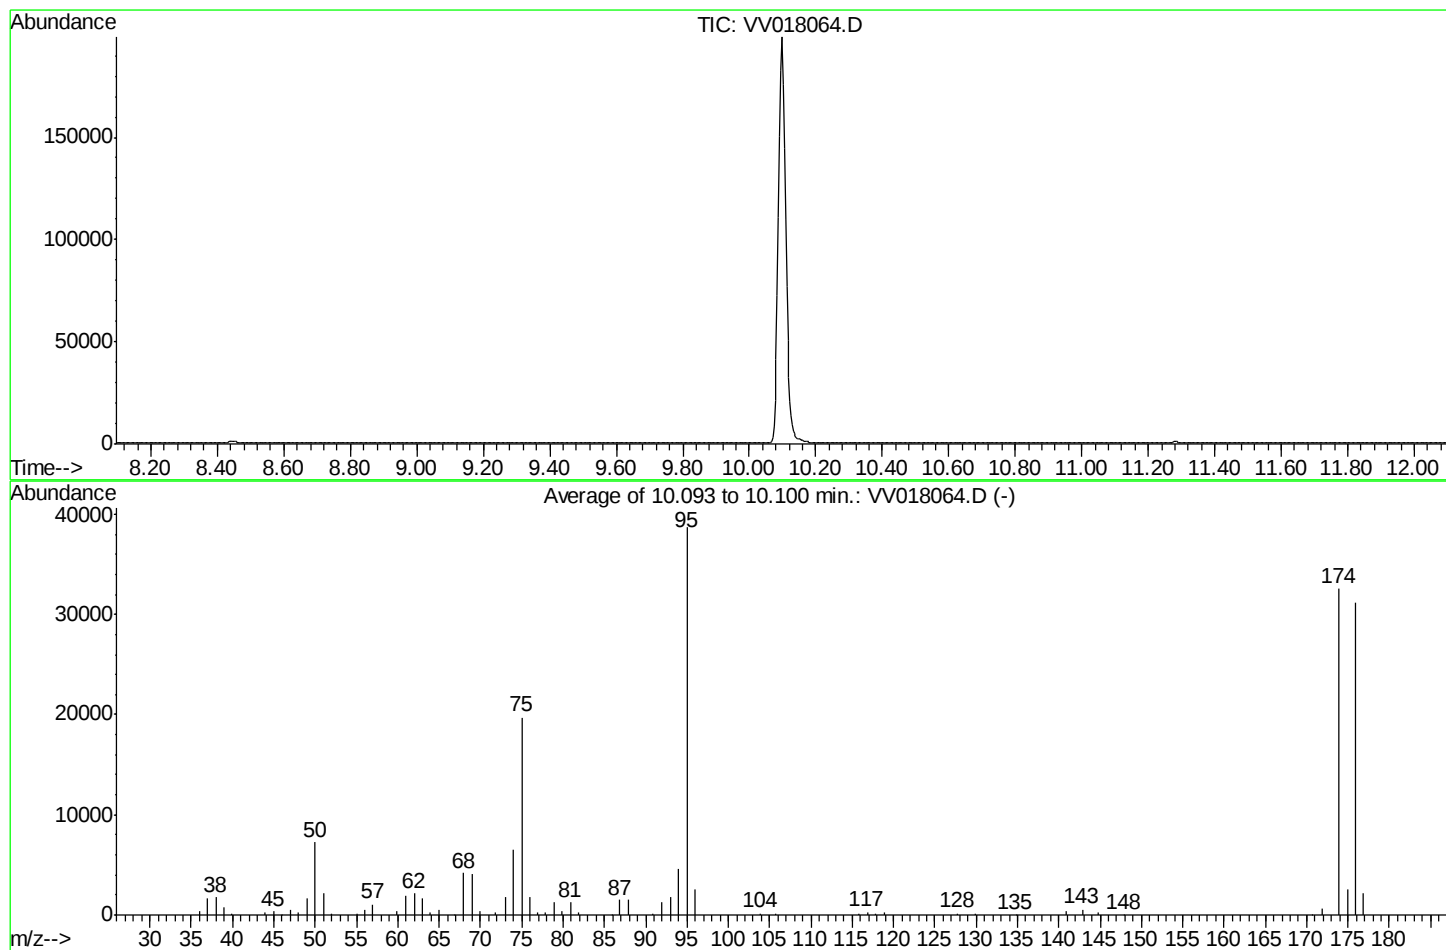

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	7268	PASS
75	95	30	80	50.9	19690	PASS
95	95	100	100	100.0	38690	PASS
96	95	5	9	6.8	2620	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.2	32570	PASS
175	174	5	9	7.9	2588	PASS
176	174	95	101	95.5	31120	PASS
177	176	5	9	6.8	2123	PASS

m/z	Abundance
35.90	337.0
37.00	1579.0
38.00	1655.0
39.00	830.0
39.90	209.0
43.90	510.0
45.00	323.0
46.90	488.0
48.00	246.0
49.00	1546.0
50.00	7146.0
51.00	2050.0
52.10	106.0
55.00	118.0
56.00	555.0
57.00	1036.0
59.90	351.0
61.00	1904.0
62.00	2047.0
63.00	1639.0
64.00	263.0
65.00	488.0
68.00	4003.0
69.00	3909.0
70.00	304.0
71.80	215.0
73.00	1734.0
74.00	6205.0
75.00	18648.0
76.00	1668.0
76.90	205.0
77.90	200.0
78.90	1178.0
79.90	370.0
80.90	1220.0
81.90	322.0
85.90	109.0
86.90	1421.0
87.90	1509.0
90.90	118.0
92.00	1212.0
93.00	1740.0
94.00	4458.0
95.00	36968.0
96.00	2558.0
103.90	194.0
105.80	160.0
115.80	111.0
116.80	302.0
117.80	125.0
118.90	251.0
127.70	134.0
129.90	139.0
140.90	392.0
142.90	549.0
144.80	212.0
170.60	101.0
171.90	587.0
173.90	30568.0
175.00	2453.0
175.90	28928.0
176.90	1986.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
36.00	365.0
37.00	1716.0
38.00	1824.0
39.00	841.0
39.90	221.0
43.90	539.0
45.00	369.0
47.00	512.0
48.00	253.0
49.00	1668.0
50.00	7450.0
51.00	2217.0
52.00	115.0
55.10	129.0
56.00	582.0
57.00	1090.0
59.90	388.0
61.00	2069.0
62.00	2231.0
63.00	1776.0
63.90	278.0
65.00	542.0
68.00	4332.0
69.00	4270.0
70.00	367.0
71.80	209.0
73.00	1936.0
74.00	6778.0
75.00	20368.0
76.00	1853.0
77.00	218.0
77.90	228.0
78.90	1335.0
79.90	396.0
80.90	1302.0
81.90	320.0
86.90	1560.0
87.90	1565.0
90.80	127.0
92.00	1298.0
93.00	1930.0
94.00	4706.0
95.00	40032.0
96.00	2734.0
103.90	206.0
105.80	173.0
115.80	131.0
116.80	332.0
117.80	141.0
118.90	282.0
127.80	153.0
129.90	139.0
140.90	405.0
142.90	604.0
144.80	214.0
171.90	647.0
173.90	33600.0
175.00	2688.0
175.90	32176.0
176.90	2210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	351.0
37.00	1673.0
38.00	1820.0
39.00	781.0
39.90	207.0
43.90	557.0
44.90	390.0
46.00	101.0
47.00	512.0
47.90	259.0
49.00	1670.0
50.00	7208.0
51.00	2177.0
51.90	141.0
55.10	135.0
56.00	556.0
57.00	1013.0
59.90	374.0
61.00	1976.0
62.00	2125.0
63.00	1699.0
63.90	267.0
65.00	541.0
66.80	109.0
68.00	4170.0
69.00	4124.0
69.90	364.0
71.90	218.0
73.00	1892.0
74.00	6741.0
75.00	20056.0
76.00	1901.0
77.00	229.0
77.90	221.0
78.90	1365.0
79.90	421.0
80.90	1298.0
81.90	298.0
86.90	1604.0
87.90	1480.0
90.90	148.0
92.00	1283.0
93.00	1903.0
94.00	4515.0
95.00	39072.0
96.00	2568.0
103.90	185.0
105.80	170.0
115.80	141.0
116.80	328.0
117.80	149.0
118.90	269.0
127.80	175.0
129.90	141.0
134.80	108.0
141.00	396.0
142.90	586.0
144.80	196.0
147.90	103.0
171.90	630.0
173.90	33544.0
175.00	2623.0
175.90	32256.0
176.90	2173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Scan 2790 (10.061 min): VV018064.D
BFB78

m/z	Abundance
39.90	133.0
43.90	326.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78