

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082021\
 Data File : VV021905.D
 Acq On : 20 Aug 2021 10:31
 Operator : SY/MD
 Sample : VV0820WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 21 00:53:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 21 00:50:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	413212	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	384461	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	185403	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	125891	38.971	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.940%
7) Chloroethane-d5	1.558	69	103239	42.351	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.700%
11) 1,1-Dichloroethene-d2	2.105	63	159728	31.063	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.120%
21) 2-Butanone-d5	3.876	46	207107	103.086	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.090%
24) Chloroform-d	4.352	84	248304	44.366	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.740%
26) 1,2-Dichloroethane-d4	5.034	65	150361	46.706	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.420%
32) Benzene-d6	5.053	84	519835	47.020	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.040%
36) 1,2-Dichloropropane-d6	6.072	67	163994	47.633	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.260%
41) Toluene-d8	7.320	98	469084	45.905	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.800%
43) trans-1,3-Dichloroprop...	7.625	79	73040	43.107	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.220%
47) 2-Hexanone-d5	8.088	63	111449	98.767	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.770%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	212985	49.921	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.840%
66) 1,2-Dichlorobenzene-d4	11.625	152	189133	49.292	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.580%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.625	75	3457	0.773	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082021\
Data File : VV021905.D
Acq On : 20 Aug 2021 10:31
Operator : SY/MD
Sample : VV0820WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :

Quant Time: Aug 21 00:53:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 21 00:50:00 2021
Response via : Initial Calibration

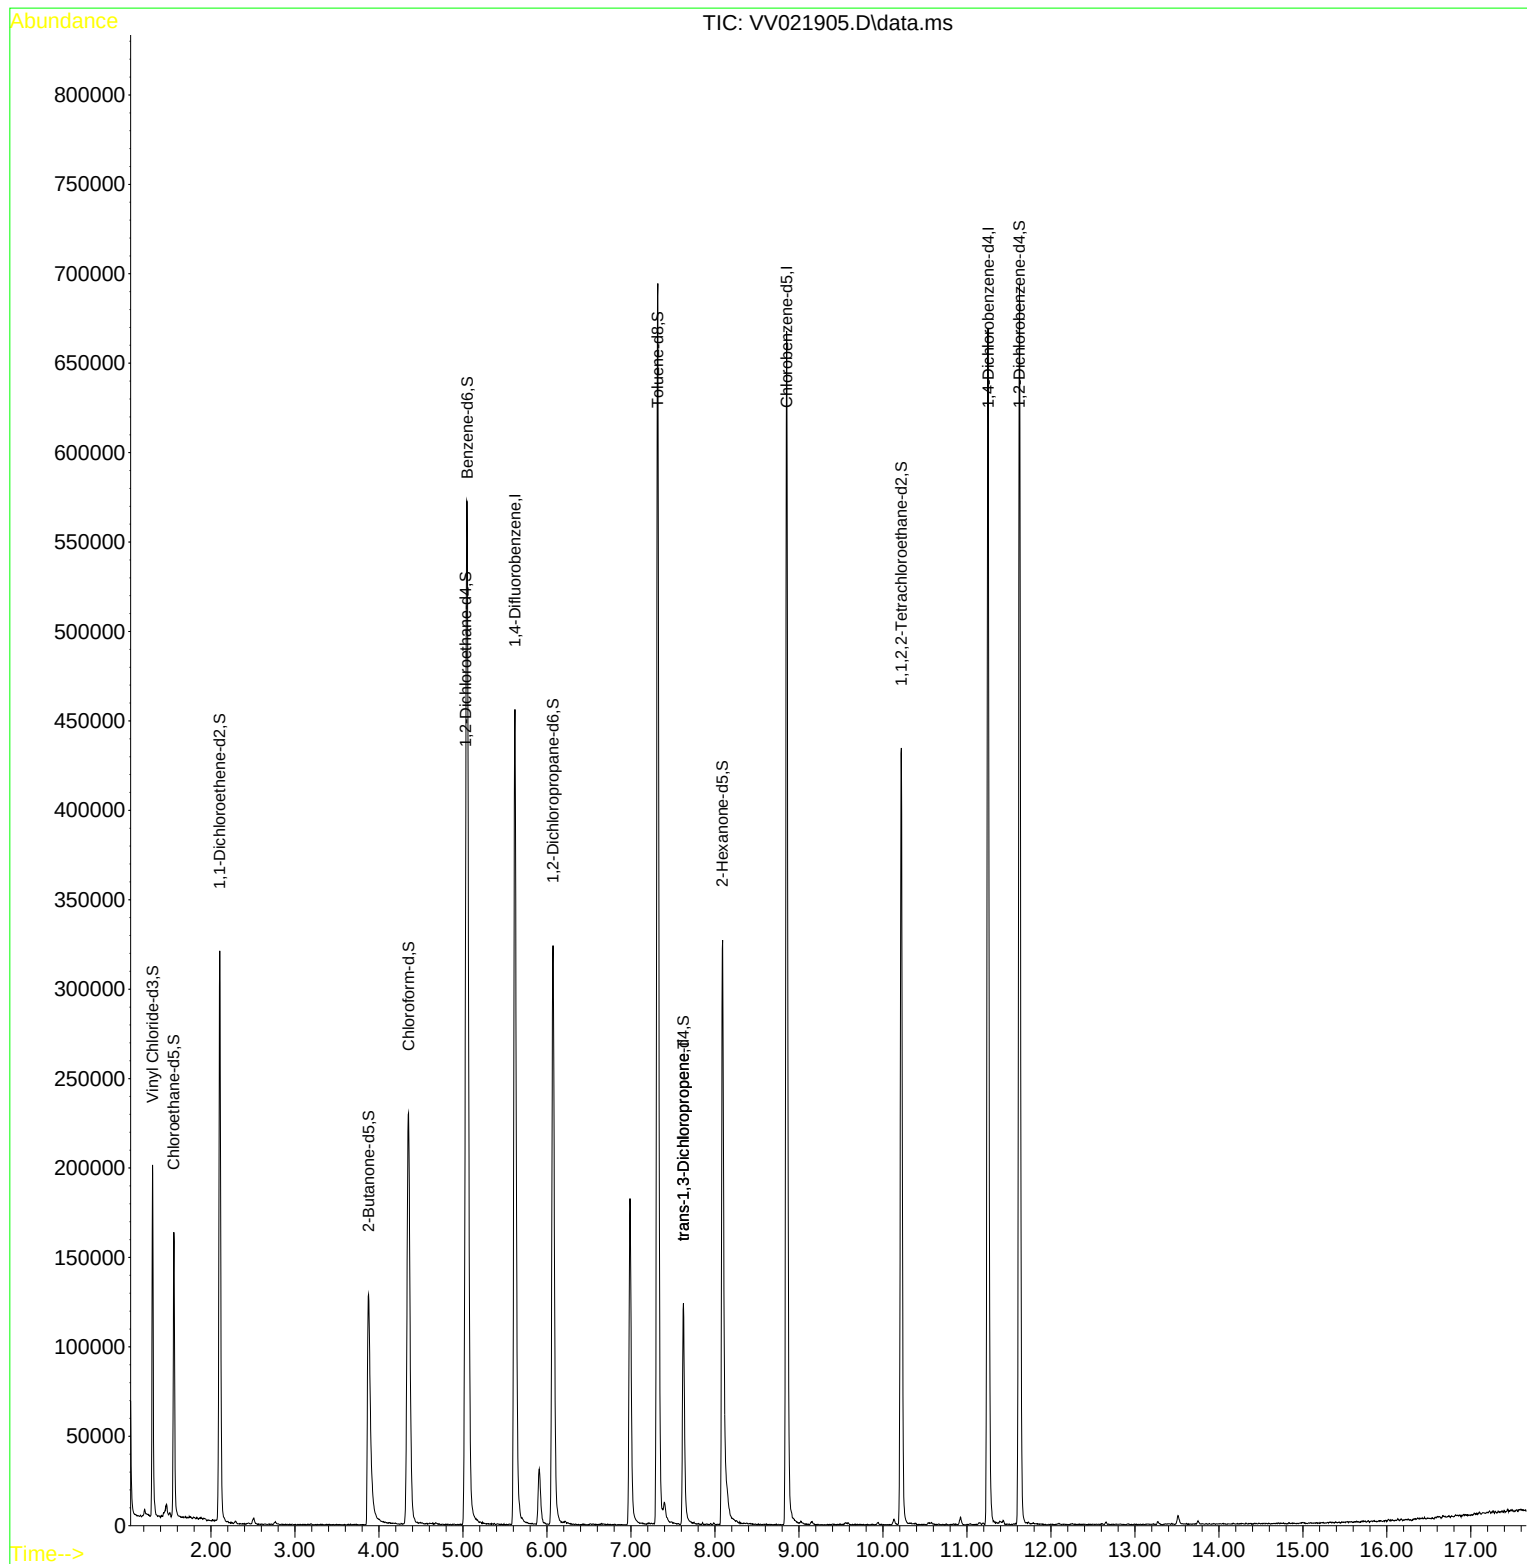

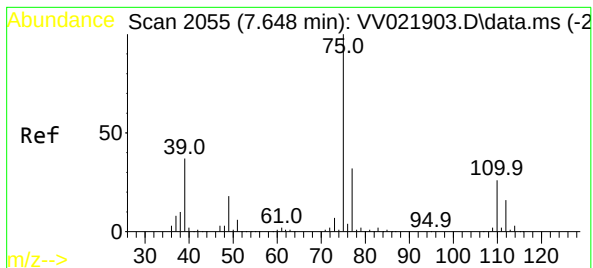

#44
 trans-1,3-Dichloropropene
 Concen: 0.773 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.022 min
 Lab File: VV021905.D
 Acq: 20 Aug 2021 10:31

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3457
 Ion Ratio Lower Upper
 75 100
 77 50.9 22.2 41.2#

