

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082021\
 Data File : VV021908.D
 Acq On : 20 Aug 2021 12:37
 Operator : SY/MD
 Sample : M3464-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKF4

Quant Time: Aug 21 00:53:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 21 00:50:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	395771	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	361833	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	170176	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	114805	37.106	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.220%
7) Chloroethane-d5	1.558	69	98329	42.114	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.220%
11) 1,1-Dichloroethene-d2	2.101	63	154787	31.429	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.860%
21) 2-Butanone-d5	3.873	46	206184	107.149	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.150%
24) Chloroform-d	4.349	84	242465	45.232	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.460%
26) 1,2-Dichloroethane-d4	5.031	65	147333	47.782	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.560%
32) Benzene-d6	5.050	84	506164	48.646	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.300%
36) 1,2-Dichloropropane-d6	6.072	67	160373	49.494	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.980%
41) Toluene-d8	7.317	98	458133	47.637	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.280%
43) trans-1,3-Dichloroprop...	7.625	79	68723	43.096	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.200%
47) 2-Hexanone-d5	8.092	63	110222	103.789	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.790%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	199778	49.753	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.500%
66) 1,2-Dichlorobenzene-d4	11.625	152	180091	51.135	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.280%
Target Compounds					Qvalue	
13) Acetone	2.159	43	4376	2.764	ug/L	# 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082021\
Data File : VV021908.D
Acq On : 20 Aug 2021 12:37
Operator : SY/MD
Sample : M3464-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKF4


Quant Time: Aug 21 00:53:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 21 00:50:00 2021
Response via : Initial Calibration

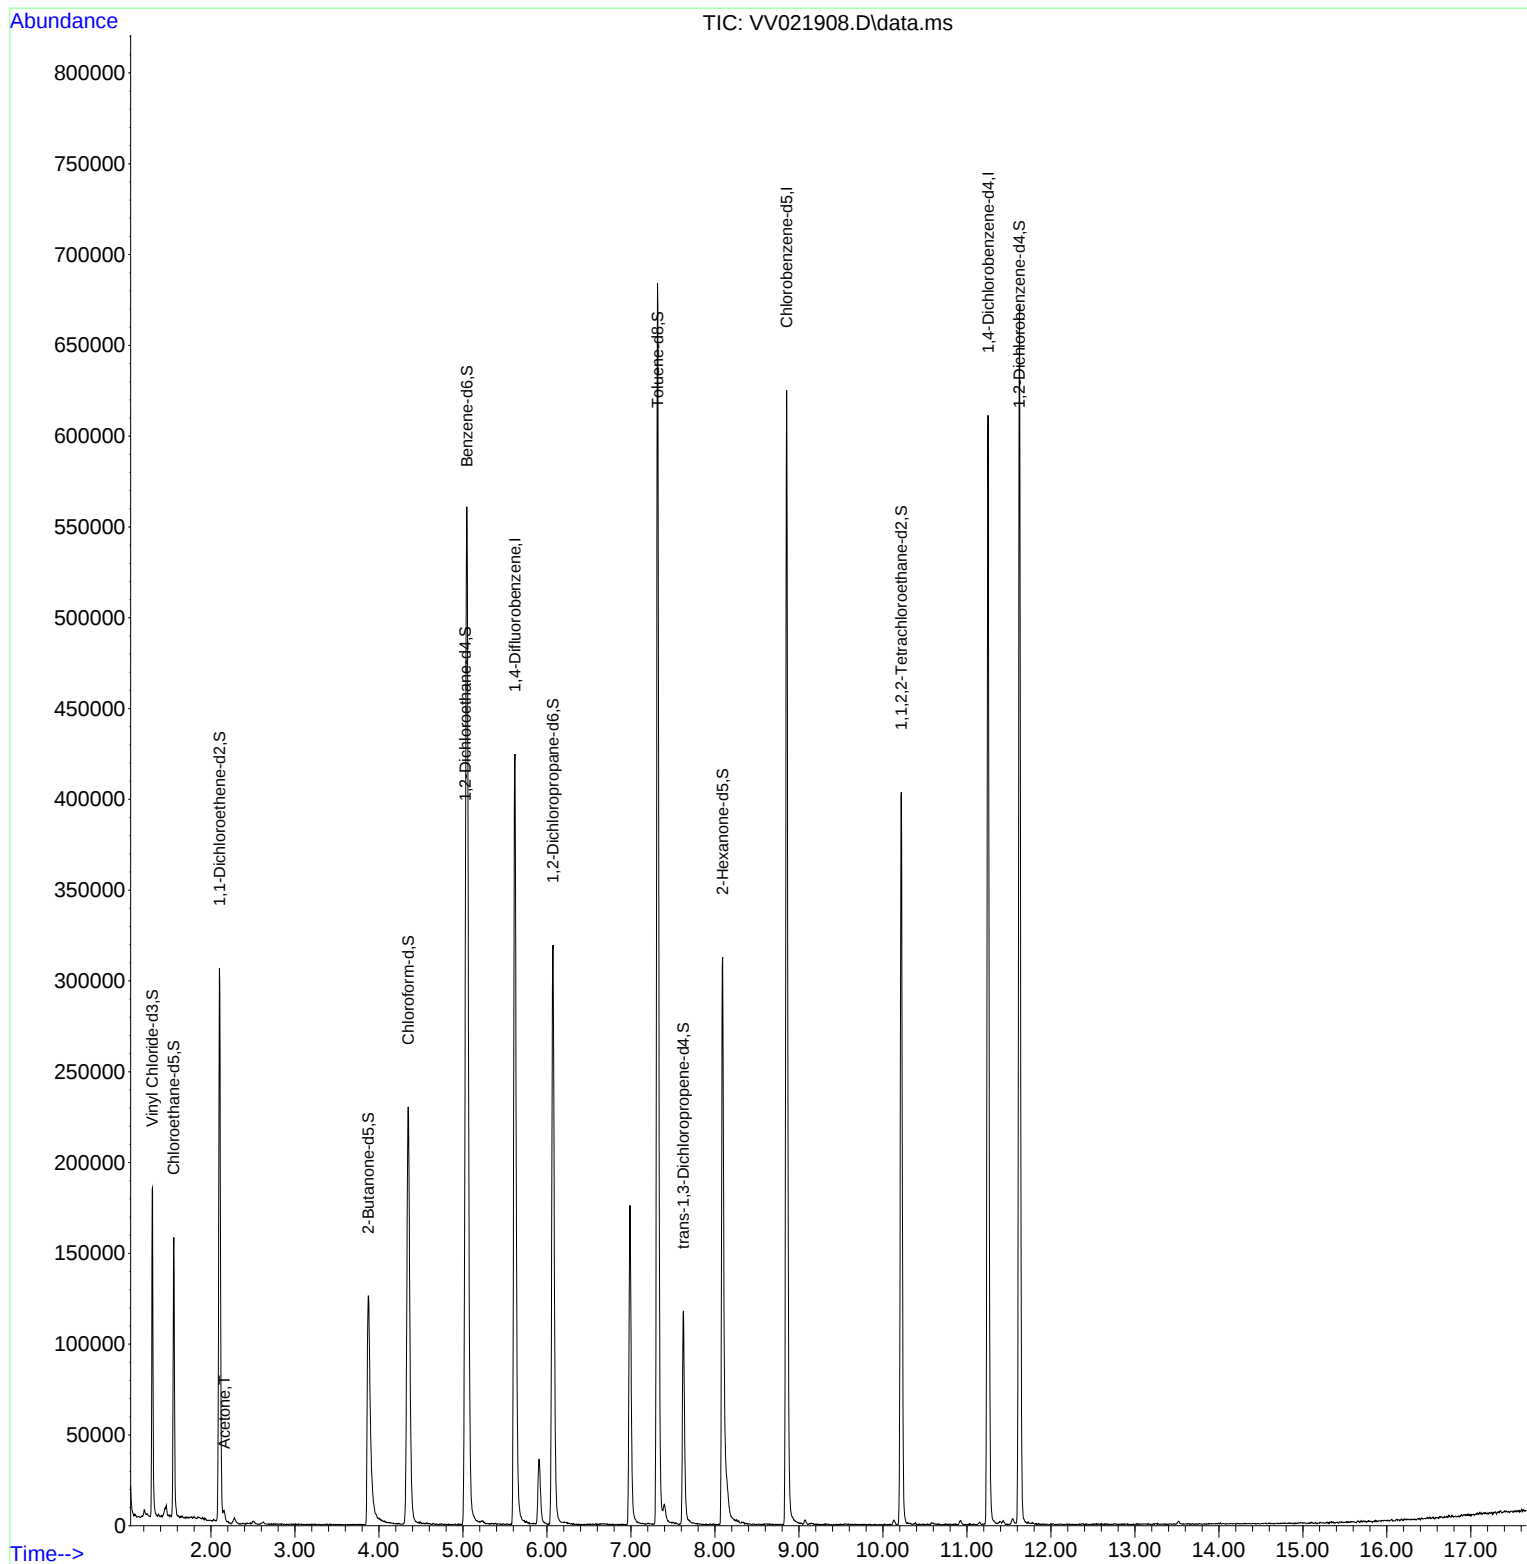

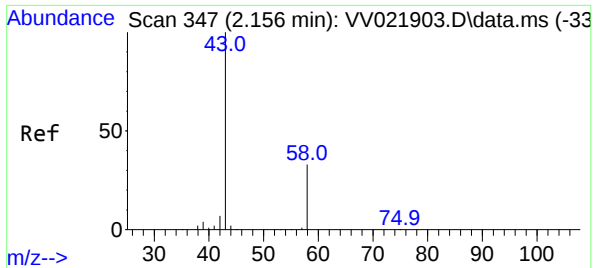

#13
 Acetone
 Concen: 2.764 ug/L
 RT: 2.159 min Scan# 348
 Delta R.T. 0.003 min
 Lab File: VV021908.D
 Acq: 20 Aug 2021 12:37

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKF4

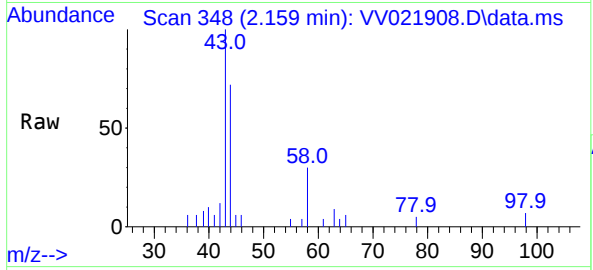

Tgt Ion: 43 Resp: 4376
 Ion Ratio Lower Upper
 43 100
 58 29.5 0.0 0.0#

