


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082021\
 Data File : VV021902.D
 Acq On : 20 Aug 2021 08:56
 Operator : SY/MD
 Sample : BFB219
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB219

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 21 00:50:00 2021

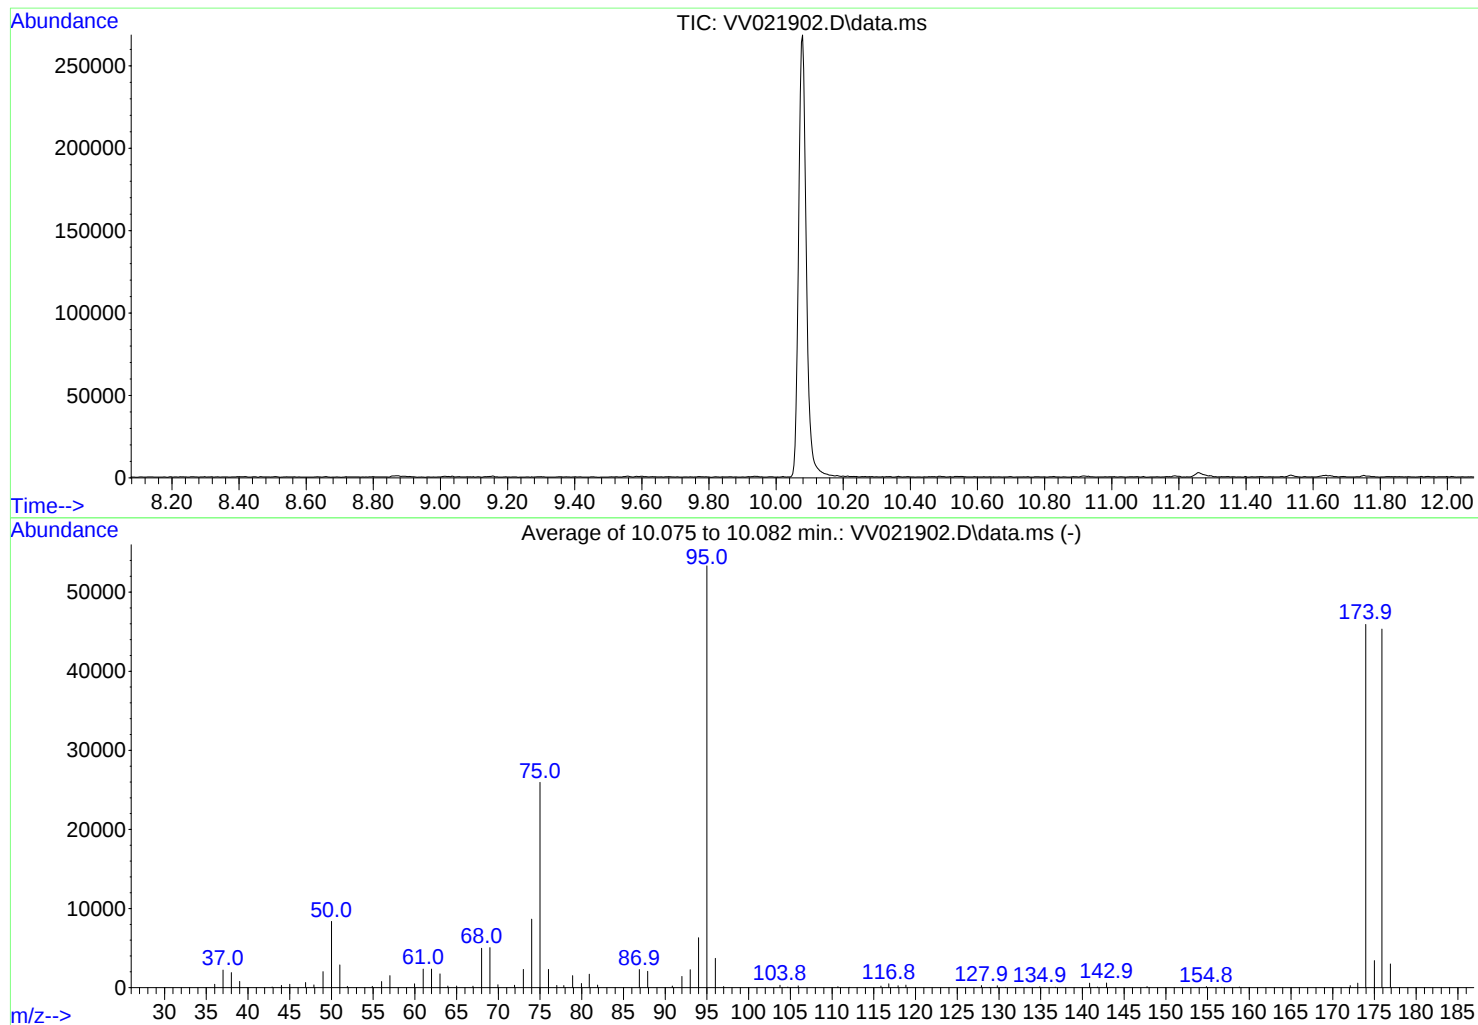

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	8367	PASS
75	95	30	80	48.7	25952	PASS
95	95	100	100	100.0	53325	PASS
96	95	5	9	6.9	3706	PASS
173	174	0.00	2	1.2	564	PASS
174	95	50	120	86.1	45925	PASS
175	174	5	9	7.4	3410	PASS
176	174	95	105	98.7	45325	PASS
177	176	5	10	6.6	2996	PASS

m/z	Abundance
36.00	449.0
37.00	2332.0
38.00	1997.0
39.00	795.0
39.80	193.0
42.90	104.0
44.00	682.0
45.00	438.0
46.90	665.0
47.90	343.0
49.00	2105.0
50.00	8545.0
51.00	3043.0
51.90	174.0
54.90	189.0
56.00	804.0
57.00	1578.0
60.00	505.0
61.00	2430.0
62.00	2445.0
63.00	1804.0
63.90	219.0
65.00	212.0
66.90	185.0
68.00	5079.0
69.00	5273.0
69.90	368.0
71.90	327.0
73.00	2395.0
74.00	8919.0
75.00	26832.0
76.00	2371.0
77.00	301.0
77.90	266.0
78.90	1541.0
79.90	556.0
80.90	1784.0
81.90	339.0
86.90	2310.0
87.90	2092.0
90.80	192.0
92.00	1453.0
93.00	2377.0
94.00	6484.0
95.00	54976.0
96.00	3848.0
97.00	159.0
103.70	316.0
104.70	117.0
106.00	229.0
110.70	127.0
115.80	209.0
116.80	516.0
117.90	260.0
118.90	321.0
127.90	284.0
129.80	249.0
134.90	121.0
136.80	106.0
140.80	559.0
141.80	113.0
142.90	601.0
147.70	129.0
154.90	141.0
158.80	108.0
172.10	298.0
173.00	583.0
174.00	47416.0
175.00	3561.0
175.90	46800.0
176.90	3102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
40.00	184.0
44.00	365.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
36.00	466.0
37.00	2278.0
38.00	1853.0
39.00	803.0
39.80	214.0
42.90	131.0
44.00	643.0
45.00	448.0
46.90	709.0
47.90	401.0
49.00	2071.0
50.00	8766.0
51.00	2784.0
51.90	153.0
54.90	182.0
56.00	862.0
57.00	1505.0
59.90	473.0
61.00	2561.0
62.00	2340.0
63.00	1785.0
63.90	225.0
65.00	219.0
66.90	182.0
68.00	5326.0
69.00	5327.0
70.00	355.0
71.90	331.0
73.00	2477.0
74.00	8788.0
75.00	26784.0
76.00	2341.0
77.10	253.0
77.90	297.0
78.90	1663.0
80.00	552.0
80.90	1738.0
81.90	362.0
86.90	2199.0
87.90	2145.0
90.80	217.0
92.00	1442.0
93.00	2050.0
94.00	6473.0
95.00	54528.0
96.00	3687.0
97.00	155.0
103.80	323.0
104.70	131.0
105.90	233.0
110.70	101.0
115.90	191.0
116.80	482.0
117.90	268.0
118.80	305.0
127.90	305.0
128.90	115.0
129.70	262.0
130.80	103.0
134.80	100.0
136.70	106.0
140.80	500.0
141.80	108.0
142.90	572.0
147.70	157.0
154.80	115.0
156.70	119.0
172.10	275.0
173.00	568.0
173.90	45848.0
175.00	3323.0
175.90	45048.0
176.90	3095.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
36.00	369.0
37.00	2045.0
38.00	1857.0
39.00	746.0
39.90	203.0
44.00	650.0
45.00	419.0
46.90	542.0
47.90	301.0
49.00	1903.0
50.00	7790.0
51.00	2807.0
51.90	137.0
54.90	148.0
56.00	648.0
57.00	1449.0
60.00	485.0
61.00	2036.0
62.00	2243.0
63.00	1637.0
64.00	182.0
65.00	189.0
67.00	185.0
68.00	4513.0
69.00	4597.0
69.90	346.0
72.00	282.0
73.00	2052.0
74.00	8242.0
75.00	24240.0
76.00	2209.0
76.90	320.0
77.80	215.0
78.90	1333.0
79.90	464.0
80.90	1597.0
81.90	299.0
86.90	2364.0
87.90	1981.0
90.90	192.0
92.00	1386.0
93.00	2403.0
94.00	5964.0
95.00	50472.0
96.00	3583.0
97.00	130.0
103.80	300.0
106.00	209.0
110.70	111.0
112.10	117.0
115.80	202.0
116.80	488.0
117.90	196.0
118.90	324.0
127.90	217.0
129.90	215.0
135.00	144.0
140.90	630.0
142.90	600.0
147.80	121.0
154.80	152.0
158.80	109.0
172.10	242.0
173.00	540.0
174.00	44512.0
175.00	3346.0
175.90	44128.0
176.90	2791.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219