

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
 Data File : VV036983.D
 Acq On : 20 Aug 2024 11:57
 Operator : SY/MD
 Sample : P3593-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 21 02:06:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 21 02:05:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	631199	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	608810	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	288035	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	223014	44.236	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.480%		
7) Chloroethane-d5	1.532	69	191695	48.216	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.440%		
11) 1,1-Dichloroethene-d2	2.059	65	101387	47.015	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.020%		
21) 2-Butanone-d5	3.793	46	201748	75.529	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	75.530%		
24) Chloroform-d	4.239	84	426659	47.160	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.320%		
26) 1,2-Dichloroethane-d4	4.934	65	273142	46.957	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.920%		
32) Benzene-d6	4.950	84	857494	46.633	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.260%		
36) 1,2-Dichloropropane-d6	5.982	67	278450	46.938	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.880%		
41) Toluene-d8	7.236	98	754626	44.738	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.480%		
43) trans-1,3-Dichloroprop...	7.548	79	116305	37.671	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.340%		
47) 2-Hexanone-d5	8.021	63	122497	71.816	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	71.820%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	296743	43.565	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.120%		
66) 1,2-Dichlorobenzene-d4	11.554	152	274703	46.803	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.600%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.059	101	3170	0.759	ug/L	# 26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
Data File : VV036983.D
Acq On : 20 Aug 2024 11:57
Operator : SY/MD
Sample : P3593-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 21 02:06:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 21 02:05:44 2024
Response via : Initial Calibration

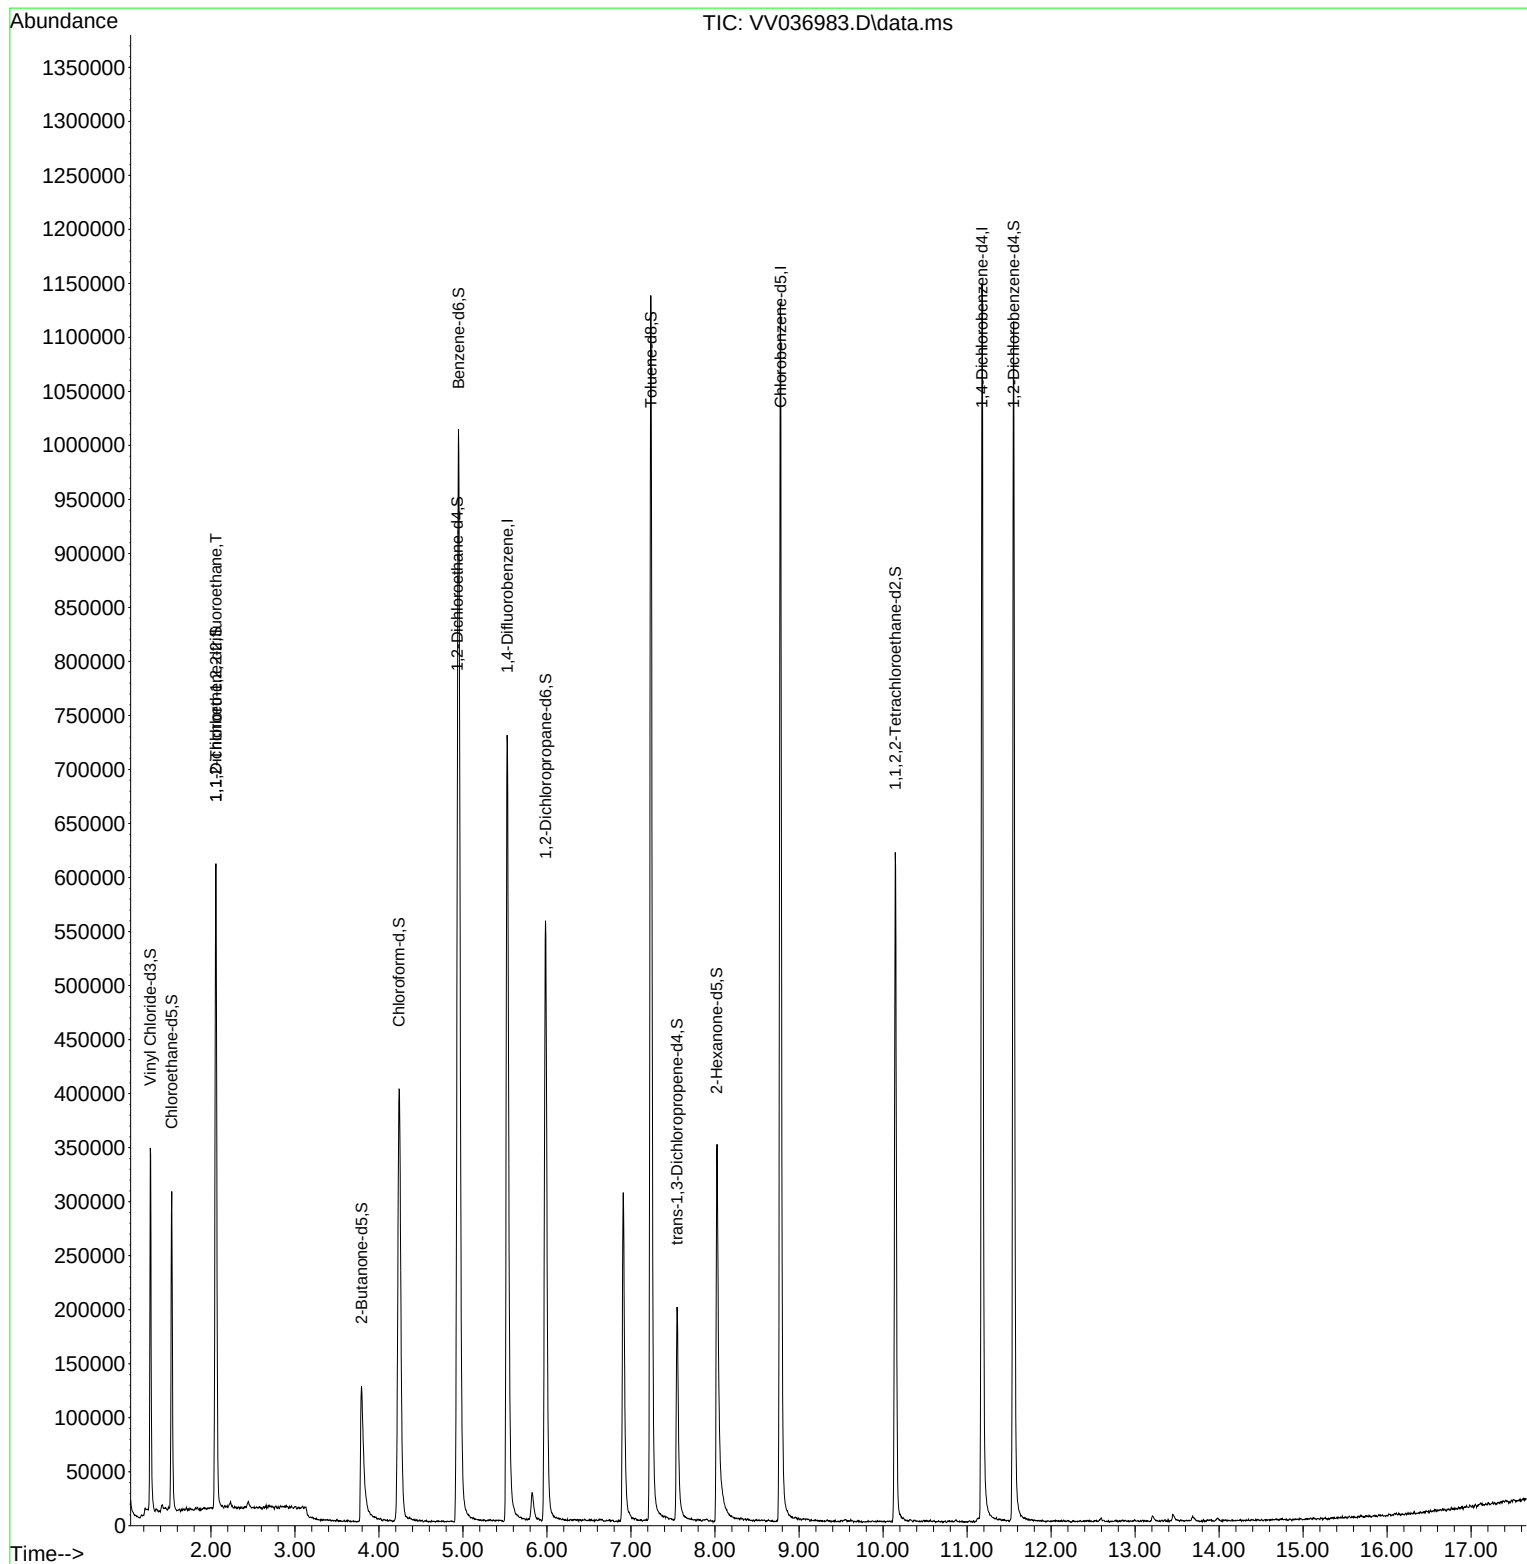

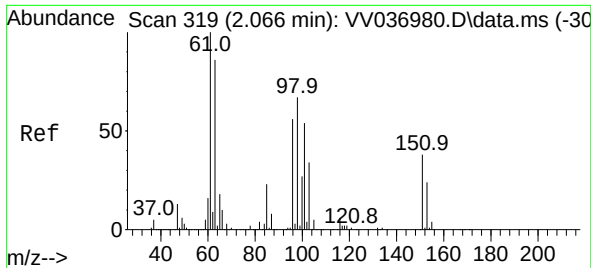

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.759 ug/L
 RT: 2.059 min Scan# 317
 Delta R.T. -0.006 min
 Lab File: VV036983.D
 Acq: 20 Aug 2024 11:57

Instrument :
 MSVOA_V
 ClientSampleId :

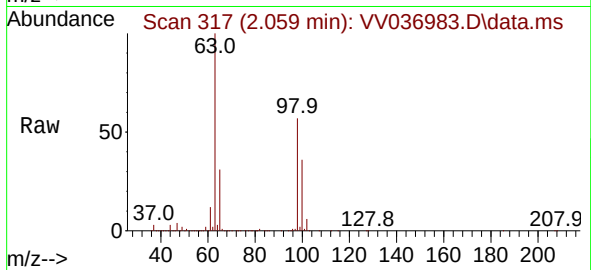

Tgt Ion:	101	Resp:	3170
Ion	Ratio	Lower	Upper
101	100		
85	7.9	34.6	51.8#
151	0.0	55.9	83.9#

