

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
 Data File : VV036982.D
 Acq On : 20 Aug 2024 11:16
 Operator : SY/MD
 Sample : VV0820WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	94	rVB	320961	349507	13.63%	1.892%
2	1.532	147	153	168	rVB	284104	335593	13.09%	1.817%
3	2.060	308	317	332	rBV	582892	836929	32.64%	4.530%
4	3.674	817	819	821	rBV2	1304	752	0.03%	0.004%
5	3.709	827	830	836	rBV8	1359	1273	0.05%	0.007%
6	3.748	840	842	846	rBV3	1016	515	0.02%	0.003%
7	3.796	849	857	886	rBV	131358	365620	14.26%	1.979%
8	4.133	959	962	964	rBV3	1605	1188	0.05%	0.006%
9	4.246	983	997	1029	rVB	400837	1011938	39.47%	5.478%
10	4.503	1074	1077	1078	rBV3	1093	580	0.02%	0.003%
11	4.648	1119	1122	1125	rVB5	1558	1034	0.04%	0.006%
12	4.683	1131	1133	1134	rBV	1046	425	0.02%	0.002%
13	4.712	1139	1142	1145	rVB4	1016	652	0.03%	0.004%
14	4.789	1164	1166	1167	rBV2	945	317	0.01%	0.002%
15	4.815	1171	1174	1176	rVB3	1007	564	0.02%	0.003%
16	4.950	1201	1216	1252	rBV2	1011137	2564091	100.00%	13.880%
17	5.397	1350	1355	1359	rBV7	1744	1717	0.07%	0.009%
18	5.532	1385	1397	1427	rBV	727705	1491815	58.18%	8.076%
19	5.985	1526	1538	1569	rBV	566780	1163100	45.36%	6.296%
20	6.754	1774	1777	1782	rBV5	1621	1829	0.07%	0.010%
21	6.841	1801	1804	1807	rBV4	1607	827	0.03%	0.004%
22	6.863	1807	1811	1813	rBV4	1475	959	0.04%	0.005%
23	6.911	1813	1826	1851	rBV	308728	594126	23.17%	3.216%
24	7.239	1917	1928	1968	rBV	1137411	2038586	79.51%	11.035%
25	7.551	2016	2025	2054	rBV	196017	369486	14.41%	2.000%
26	7.956	2148	2151	2156	rBV7	1590	1331	0.05%	0.007%
27	7.979	2156	2158	2159	rBV2	617	213	0.01%	0.001%
28	8.024	2164	2172	2221	rBV	360268	787703	30.72%	4.264%
29	8.689	2375	2379	2382	rBV5	1694	1287	0.05%	0.007%
30	8.780	2395	2407	2442	rBV	1132995	1879631	73.31%	10.175%
31	9.207	2539	2540	2545	rVB5	1432	825	0.03%	0.004%
32	9.271	2558	2560	2562	rVB3	879	425	0.02%	0.002%
33	9.291	2562	2566	2568	rBV5	1167	694	0.03%	0.004%
34	9.310	2568	2572	2575	rBV4	1512	1468	0.06%	0.008%
35	9.487	2625	2627	2631	rBV5	1307	966	0.04%	0.005%
36	9.561	2648	2650	2651	rBV2	951	417	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
 Data File : VV036982.D
 Acq On : 20 Aug 2024 11:16
 Operator : SY/MD
 Sample : VV0820WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.661	2677	2681	2685	rBV6	1625	1240	0.05%	0.007%
38	9.789	2719	2721	2723	rBV3	547	226	0.01%	0.001%
39	9.808	2723	2727	2731	rBV4	1103	1080	0.04%	0.006%
40	9.834	2731	2735	2739	rBV6	1731	1418	0.06%	0.008%
41	9.860	2739	2743	2744	rBV4	1255	953	0.04%	0.005%
42	9.963	2771	2775	2777	rBV5	900	759	0.03%	0.004%
43	9.995	2782	2785	2791	rVB7	1534	1765	0.07%	0.010%
44	10.027	2791	2795	2798	rBV7	1487	1293	0.05%	0.007%
45	10.040	2798	2799	2802	rBV3	1218	636	0.02%	0.003%
46	10.069	2806	2808	2812	rVB4	1449	761	0.03%	0.004%
47	10.085	2812	2813	2814	rBV2	408	143	0.01%	0.001%
48	10.104	2815	2819	2821	rBV3	1244	929	0.04%	0.005%
49	10.146	2821	2832	2853	rBV	624030	997939	38.92%	5.402%
50	10.365	2898	2900	2901	rBV	1231	378	0.01%	0.002%
51	10.397	2909	2910	2912	rVB2	929	285	0.01%	0.002%
52	10.458	2926	2929	2932	rBV5	1004	709	0.03%	0.004%
53	10.683	2997	2999	3002	rBV2	996	587	0.02%	0.003%
54	10.770	3024	3026	3027	rBV2	869	324	0.01%	0.002%
55	10.821	3040	3042	3047	rVB4	1446	1018	0.04%	0.006%
56	10.853	3047	3052	3053	rBV6	1784	1323	0.05%	0.007%
57	10.931	3074	3076	3078	rBV3	1291	766	0.03%	0.004%
58	10.982	3088	3092	3094	rVB4	1284	828	0.03%	0.004%
59	10.998	3094	3097	3099	rBV3	1520	984	0.04%	0.005%
60	11.085	3120	3124	3130	rVB7	1333	1468	0.06%	0.008%
61	11.117	3130	3134	3135	rBV4	2561	1610	0.06%	0.009%
62	11.178	3143	3153	3179	rBV	1153801	1824292	71.15%	9.875%
63	11.468	3240	3243	3246	rBV4	967	847	0.03%	0.005%
64	11.554	3259	3270	3297	rBV	1130215	1813059	70.71%	9.814%
65	12.017	3411	3414	3415	rBV4	1103	591	0.02%	0.003%
66	12.275	3491	3494	3497	rBV5	1799	1093	0.04%	0.006%
67	12.291	3497	3499	3502	rBV4	957	566	0.02%	0.003%
68	12.471	3550	3555	3556	rBV4	1002	675	0.03%	0.004%
69	12.554	3578	3581	3583	rBV4	1079	626	0.02%	0.003%
70	12.699	3624	3626	3629	rBV4	1051	549	0.02%	0.003%
71	12.757	3642	3644	3645	rBV2	1056	352	0.01%	0.002%
72	12.911	3690	3692	3695	rBV4	1285	797	0.03%	0.004%
73	13.101	3749	3751	3753	rBV2	1032	604	0.02%	0.003%
74	13.355	3827	3830	3831	rBV2	1285	685	0.03%	0.004%
75	14.020	4034	4037	4038	rBV2	1249	761	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
Data File : VV036982.D
Acq On : 20 Aug 2024 11:16
Operator : SY/MD
Sample : VV0820WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis




Sum of corrected areas: 18473302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
Data File : VV036982.D
Acq On : 20 Aug 2024 11:16
Operator : SY/MD
Sample : VV0820WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

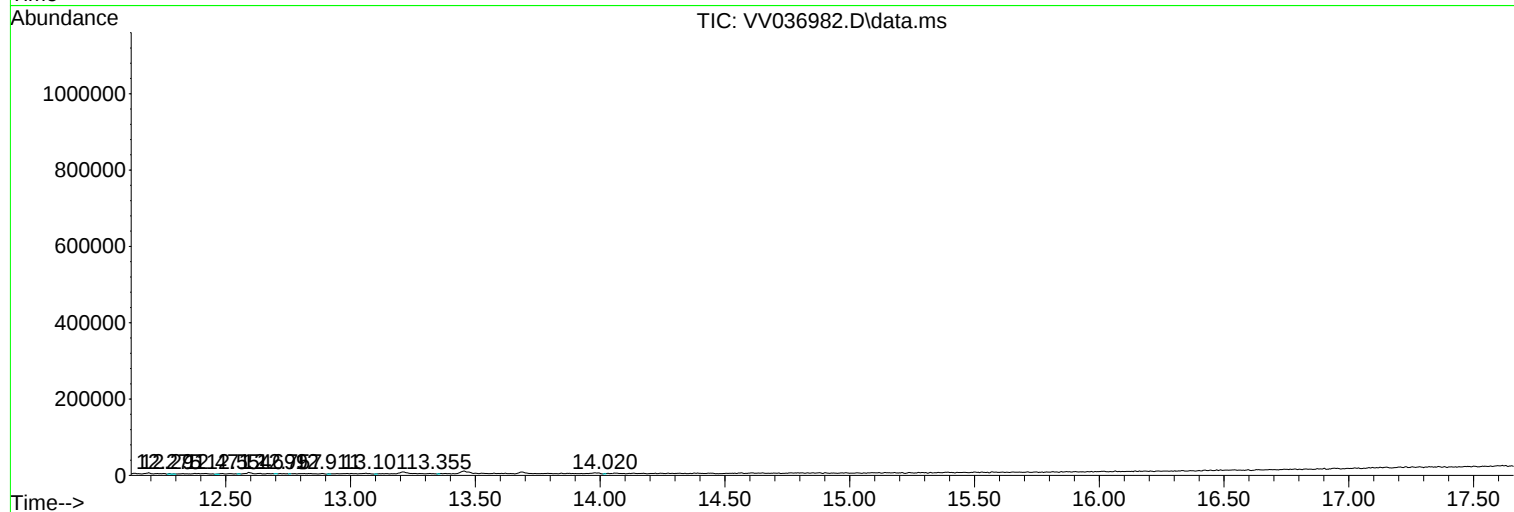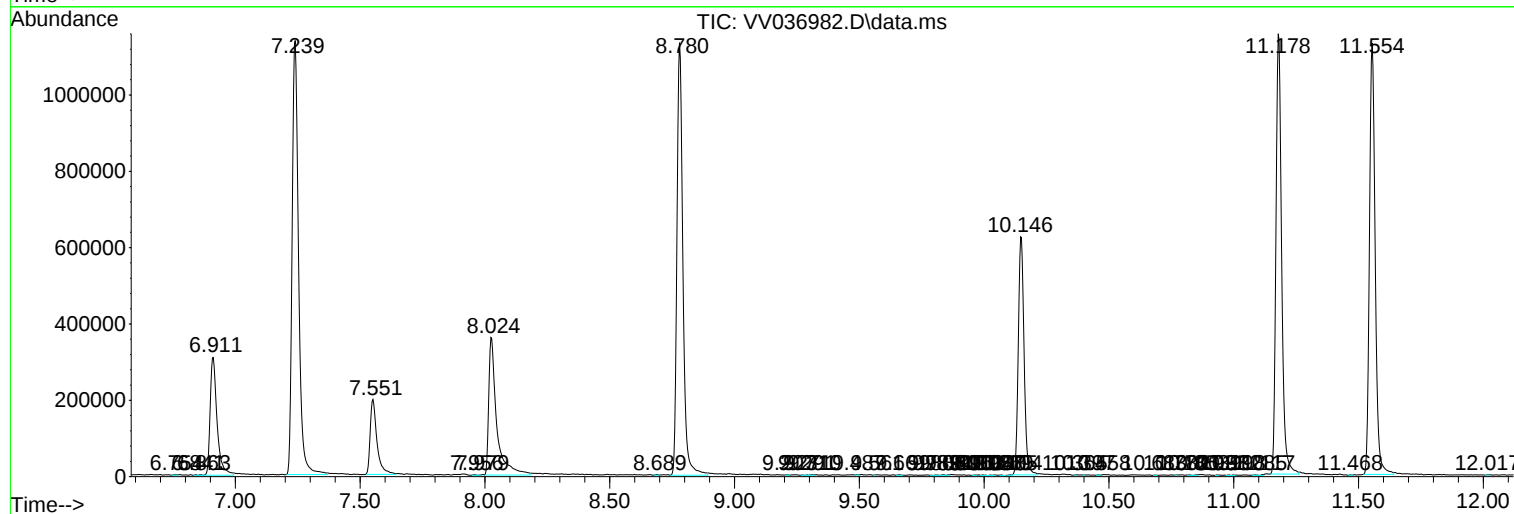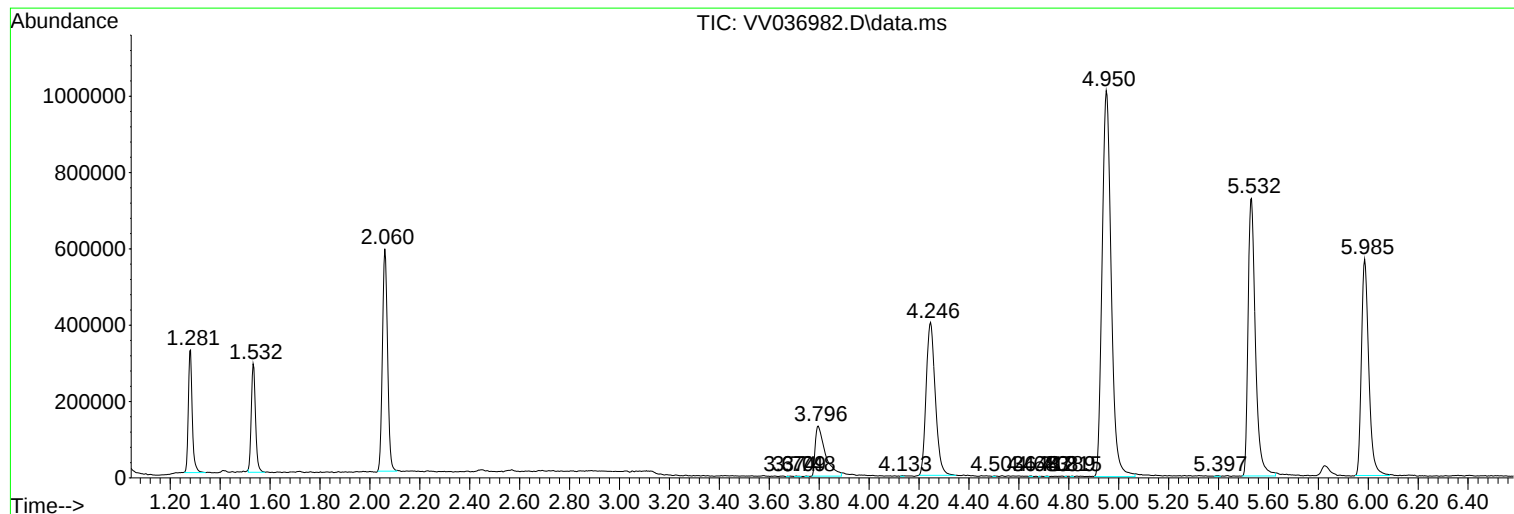

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
Data File : VV036982.D
Acq On : 20 Aug 2024 11:16
Operator : SY/MD
Sample : VV0820WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
Data File : VV036982.D
Acq On : 20 Aug 2024 11:16
Operator : SY/MD
Sample : VV0820WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
