
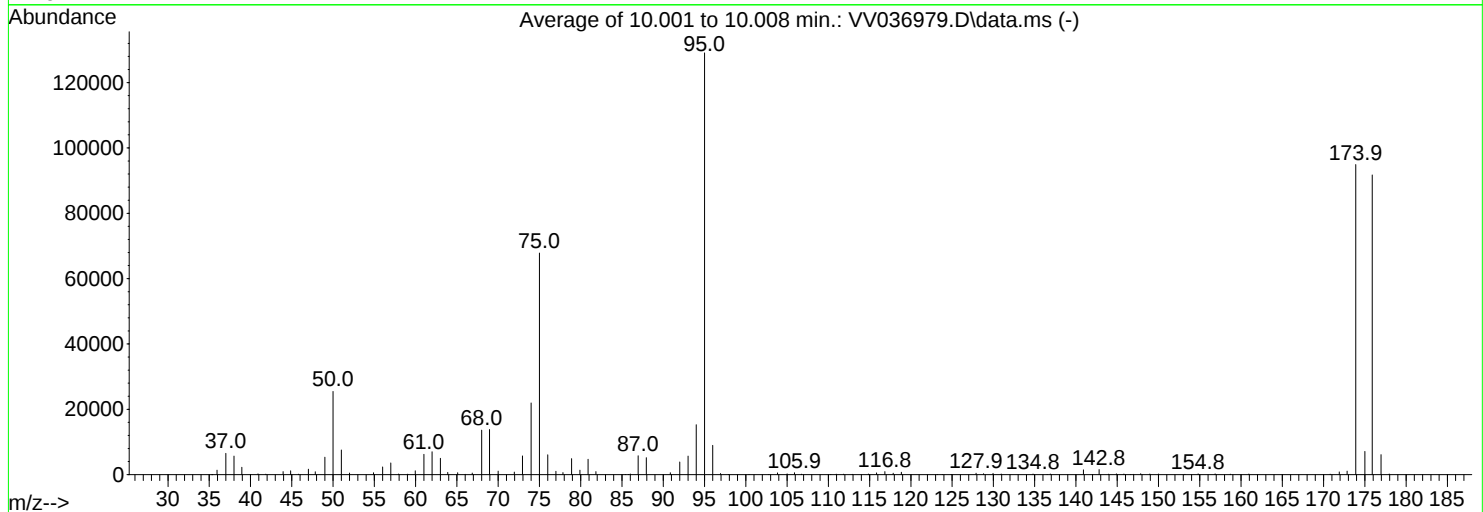


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082024\
Data File : VV036979.D
Acq On : 20 Aug 2024 08:17
Operator : SY/MD
Sample : BFB365
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB365

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Wed Aug 21 02:05:44 2024

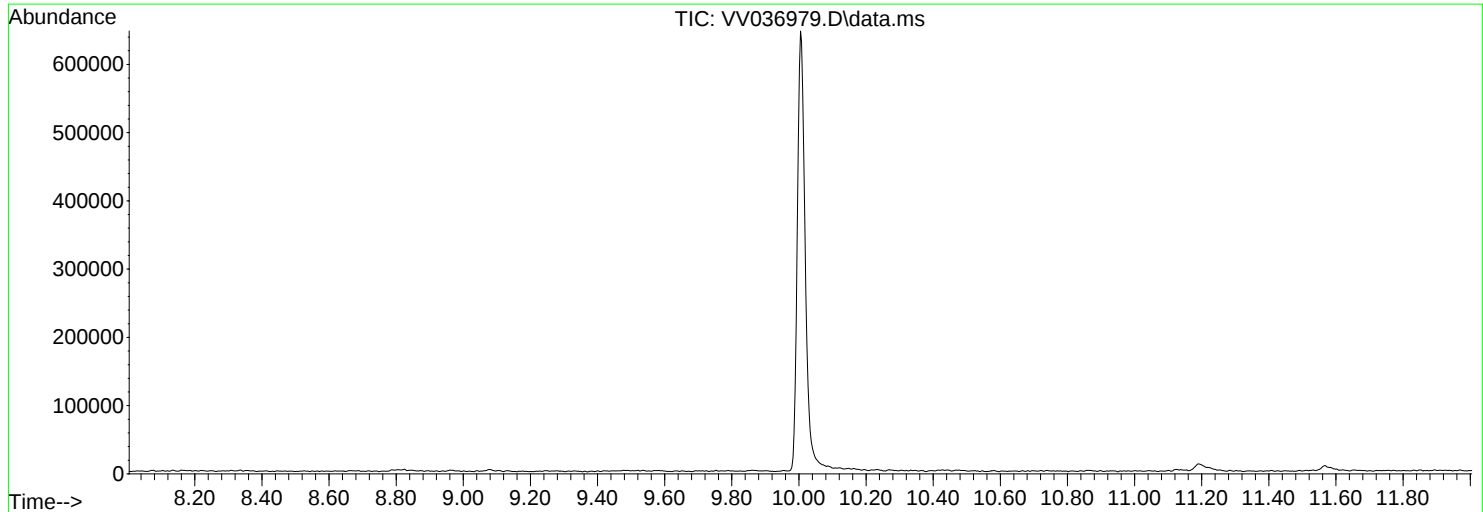

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	25488	PASS
75	95	30	80	52.5	67811	PASS
95	95	100	100	100.0	129107	PASS
96	95	5	9	7.0	8984	PASS
173	174	0.00	2	1.1	1087	PASS
174	95	50	120	73.5	94920	PASS
175	174	5	9	7.5	7117	PASS
176	174	95	105	96.6	91725	PASS
177	176	5	10	6.7	6129	PASS

m/z	Abundance
35.40	124.0
36.60	111.0
38.10	132.0
38.90	227.0
39.90	524.0
42.90	258.0
43.90	1148.0
44.80	228.0
45.90	129.0
49.20	155.0
50.30	101.0
53.10	197.0
55.20	185.0
60.10	125.0
64.20	112.0
68.90	172.0
88.10	146.0
207.10	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
35.30	178.0
35.90	1324.0
37.00	6222.0
38.00	5710.0
39.00	2522.0
39.90	531.0
40.90	276.0
41.90	157.0
42.90	231.0
44.00	2051.0
44.90	1352.0
45.80	208.0
47.00	1683.0
47.90	954.0
49.00	5188.0
50.00	24344.0
51.00	7347.0
52.00	515.0
53.00	157.0
54.90	577.0
56.00	2256.0
57.00	3678.0
58.00	185.0
59.00	134.0
59.90	1342.0
61.00	6172.0
62.00	6856.0
63.00	4906.0
63.90	739.0
65.10	485.0
66.80	463.0
68.00	12823.0
69.00	13702.0
70.00	981.0
72.00	731.0
72.90	5542.0
74.00	21048.0
75.00	65192.0
76.00	5971.0
77.10	972.0
77.80	588.0
78.90	4627.0
79.90	1279.0
80.90	4611.0
81.90	889.0
85.80	168.0
87.00	6045.0
87.90	5084.0
90.80	574.0
92.00	3630.0
93.00	5241.0
94.00	14492.0
95.00	124000.0
96.00	8990.0
97.00	271.0
102.80	132.0
103.80	519.0
105.00	227.0
105.90	565.0
106.80	178.0
110.90	167.0
111.90	141.0
112.90	120.0
114.90	186.0
115.80	564.0
116.80	951.0
118.00	368.0
118.90	792.0
123.80	122.0
128.00	454.0
128.80	424.0
130.00	340.0
131.00	211.0
134.80	152.0
136.50	112.0
136.90	172.0
140.90	1313.0
142.80	1379.0
143.90	128.0
144.90	182.0
145.80	225.0
147.00	127.0
147.80	283.0
149.00	158.0
150.00	165.0
153.20	120.0
154.90	272.0
156.90	146.0
158.70	105.0
160.90	194.0
170.80	187.0
171.90	733.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

172.80	940.0
173.90	87080.0
175.00	6550.0
175.90	85256.0
177.00	5735.0
178.00	187.0
207.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
35.30	152.0
35.90	1462.0
37.00	6811.0
38.00	6030.0
39.00	2530.0
39.90	525.0
40.90	275.0
41.90	140.0
42.90	253.0
44.00	2137.0
44.90	1420.0
45.80	255.0
47.00	1715.0
47.90	901.0
49.00	5640.0
50.00	26584.0
51.00	7814.0
52.00	560.0
53.00	187.0
54.90	654.0
56.00	2456.0
57.00	3669.0
57.90	197.0
59.10	158.0
59.90	1348.0
61.00	6438.0
62.00	7333.0
63.00	5111.0
63.90	728.0
65.10	605.0
66.00	110.0
66.90	483.0
68.00	14213.0
69.00	14519.0
70.00	1136.0
71.90	779.0
72.90	5925.0
74.00	22784.0
75.00	70320.0
76.00	6317.0
77.00	1054.0
77.90	643.0
78.90	5049.0
79.90	1460.0
80.90	4889.0
81.90	959.0
86.00	274.0
86.90	5942.0
88.00	5557.0
90.80	635.0
92.00	3995.0
93.00	5871.0
94.00	15689.0
95.00	133760.0
96.00	9317.0
96.90	306.0
97.90	101.0
103.80	563.0
105.00	225.0
105.90	620.0
106.70	133.0
110.30	112.0
110.90	128.0
111.80	133.0
112.90	126.0
114.80	213.0
115.90	554.0
116.90	950.0
117.80	422.0
118.90	743.0
123.20	103.0
124.90	122.0
127.90	457.0
128.80	322.0
129.90	404.0
131.00	189.0
134.80	222.0
136.90	214.0
140.90	1542.0
142.00	103.0
142.80	1631.0
143.90	162.0
144.90	275.0
145.80	249.0
146.70	113.0
146.90	116.0
147.90	265.0
148.90	203.0
150.00	202.0
153.20	121.0
154.80	284.0
156.90	242.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

158.70	144.0
161.00	206.0
170.80	168.0
171.90	878.0
172.90	1120.0
173.90	98440.0
175.00	7440.0
175.90	95208.0
176.90	6343.0
178.00	188.0
207.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

m/z	Abundance
35.20	107.0
36.00	1373.0
37.00	6563.0
38.00	5719.0
39.00	2343.0
39.90	478.0
40.90	226.0
41.70	102.0
41.90	103.0
43.00	277.0
44.00	2121.0
44.90	1397.0
45.80	312.0
47.00	1583.0
47.80	746.0
49.00	5658.0
50.00	25536.0
51.00	7556.0
52.00	479.0
53.00	220.0
54.90	562.0
56.00	2367.0
57.00	3436.0
57.90	170.0
59.10	163.0
60.00	1294.0
61.00	6102.0
62.00	6836.0
63.00	4938.0
63.90	645.0
65.10	618.0
66.00	148.0
66.90	497.0
68.00	13805.0
69.00	13768.0
70.00	1133.0
71.90	833.0
73.00	5770.0
74.00	21928.0
75.00	67920.0
76.00	5959.0
76.90	1096.0
77.90	654.0
78.90	5018.0
79.90	1409.0
80.90	4592.0
81.80	942.0
85.40	105.0
86.00	375.0
86.90	5357.0
87.90	5349.0
90.90	549.0
92.00	3960.0
93.00	5920.0
94.00	15658.0
95.00	129560.0
96.00	8646.0
96.90	384.0
100.40	127.0
103.90	618.0
105.00	263.0
105.90	609.0
106.70	108.0
111.00	135.0
111.80	127.0
114.80	233.0
115.80	461.0
116.90	896.0
117.80	520.0
118.80	738.0
127.80	473.0
128.70	156.0
129.90	464.0
130.80	191.0
134.80	286.0
136.90	231.0
140.90	1545.0
142.80	1694.0
144.00	150.0
144.90	297.0
145.80	193.0
146.60	113.0
147.90	286.0
148.90	196.0
150.00	201.0
154.70	235.0
156.80	294.0
158.70	167.0
161.00	216.0
170.80	107.0
171.90	924.0
172.80	1201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365

173.90	99240.0
175.00	7361.0
175.90	94712.0
176.90	6310.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB365