


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV082025\
Data File : VV038967.D
Acq On : 20 Aug 2025 07:51
Operator : SY/MD
Sample : BFB240
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB240

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM081925.M
Title : TRACE VOA SOM01.0
Last Update : Wed Aug 20 03:16:00 2025

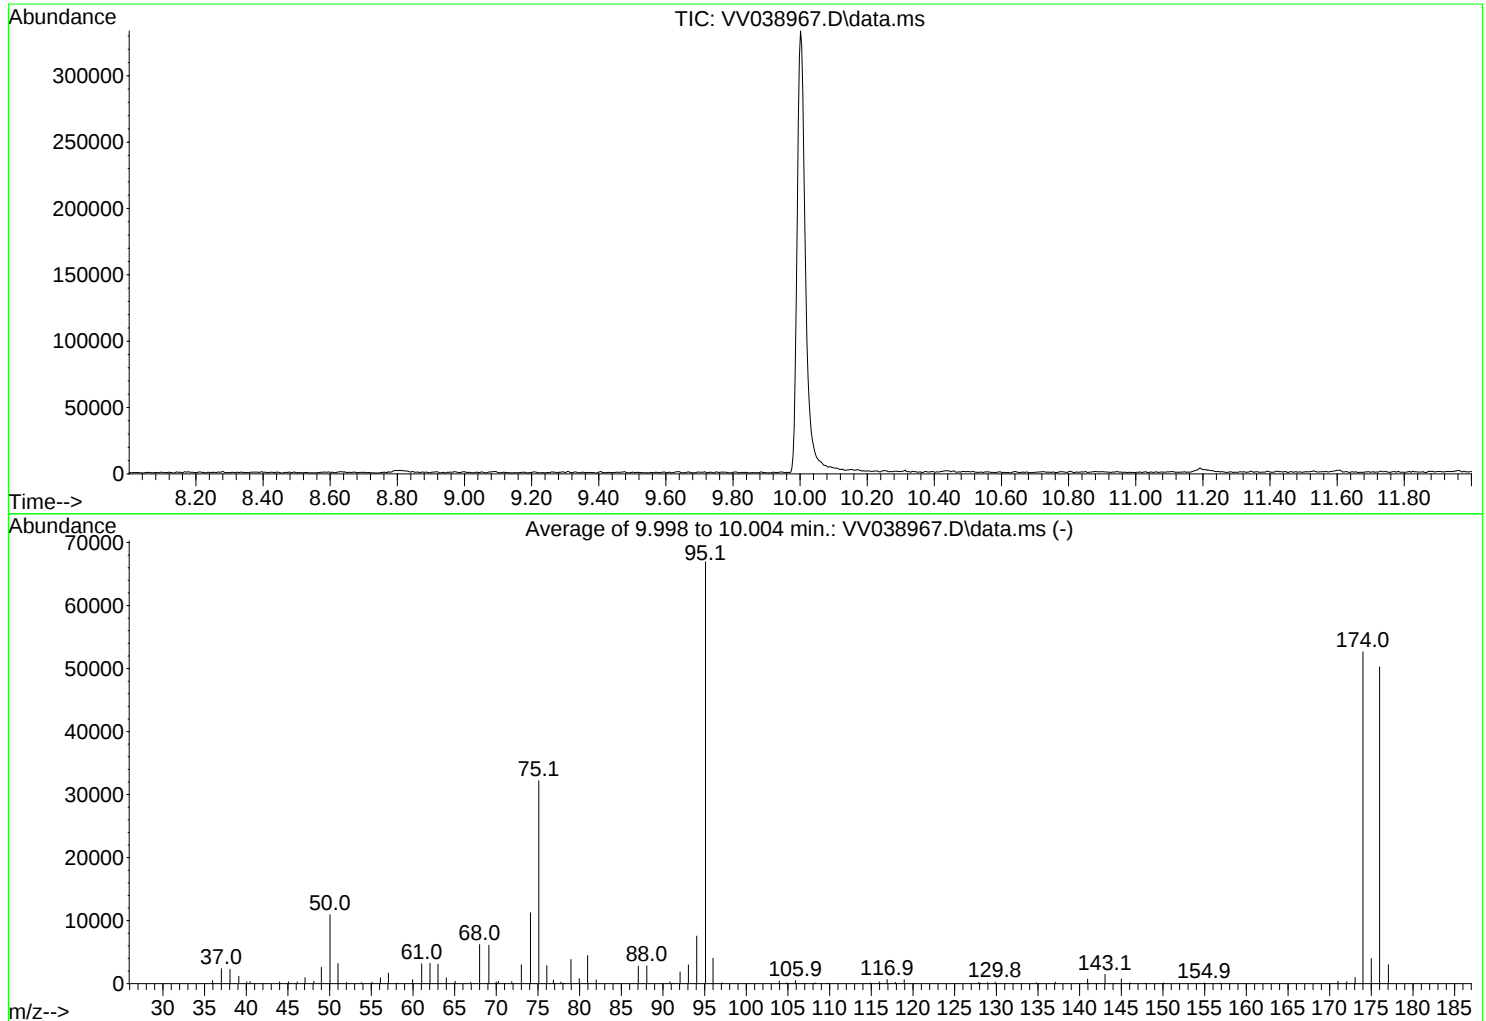

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	10941	PASS
75	95	30	80	48.1	32192	PASS
95	95	100	100	100.0	66936	PASS
96	95	5	9	6.0	4029	PASS
173	174	0.00	2	1.9	999	PASS
174	95	50	120	78.7	52659	PASS
175	174	5	9	7.6	3988	PASS
176	174	95	101	95.5	50267	PASS
177	176	5	9	6.0	3006	PASS

m/z	Abundance
39.80	203.0
44.00	771.0
76.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.00	498.0
37.00	2379.0
38.00	2248.0
39.10	1040.0
40.00	295.0
40.40	278.0
42.10	105.0
44.00	937.0
45.10	292.0
46.10	258.0
47.00	1032.0
48.10	275.0
49.00	2708.0
50.10	10755.0
51.00	3097.0
52.10	245.0
53.80	121.0
55.10	235.0
56.10	919.0
57.00	1689.0
58.10	154.0
60.00	676.0
61.00	3040.0
62.10	3291.0
63.00	3191.0
64.00	920.0
65.00	318.0
66.90	241.0
68.00	6083.0
69.10	6173.0
70.00	426.0
70.30	422.0
72.00	350.0
73.00	2937.0
74.10	10966.0
75.10	31928.0
76.10	2912.0
76.90	662.0
77.70	230.0
78.10	172.0
78.90	3833.0
79.90	854.0
80.90	4088.0
82.00	630.0
87.00	2845.0
88.10	2453.0
90.80	275.0
91.20	263.0
92.00	1747.0
93.10	3006.0
94.10	7184.0
95.10	65000.0
96.00	3982.0
97.20	145.0
103.90	372.0
104.90	125.0
105.90	437.0
108.30	213.0
114.90	158.0
116.10	291.0
116.90	672.0
117.90	166.0
118.90	556.0
127.90	331.0
128.90	111.0
129.90	243.0
134.80	163.0
137.10	249.0
141.00	777.0
143.10	1366.0
144.00	110.0
145.00	696.0
146.10	115.0
150.10	141.0
154.90	173.0
156.80	213.0
171.00	374.0
172.10	332.0
173.10	1021.0
174.00	49768.0
175.00	3767.0
176.00	48160.0
177.00	3156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
36.00	478.0
37.00	2459.0
38.10	2250.0
39.10	1222.0
40.00	292.0
40.50	357.0
44.10	1055.0
45.10	296.0
46.10	278.0
47.00	1002.0
48.10	407.0
49.00	2693.0
50.10	11272.0
51.00	3323.0
52.00	221.0
53.80	188.0
55.10	259.0
56.10	950.0
57.10	1749.0
58.10	107.0
59.90	659.0
61.00	3271.0
62.10	3299.0
63.00	3192.0
64.00	1003.0
65.10	383.0
66.90	254.0
68.00	6398.0
69.10	6221.0
70.00	325.0
70.30	400.0
71.80	340.0
73.00	3089.0
74.10	11711.0
75.10	33392.0
76.10	2910.0
76.90	730.0
77.80	286.0
79.00	3954.0
80.00	831.0
80.90	4646.0
82.00	580.0
87.10	2780.0
88.00	2937.0
90.80	278.0
92.00	1863.0
93.10	3089.0
94.10	7780.0
95.10	69032.0
96.00	4105.0
97.00	116.0
103.90	451.0
104.80	110.0
105.90	528.0
108.20	162.0
109.70	112.0
114.90	153.0
115.90	293.0
116.90	681.0
117.90	214.0
119.00	612.0
127.90	286.0
128.90	193.0
129.80	252.0
134.80	171.0
137.10	225.0
141.00	728.0
143.10	1542.0
145.00	775.0
146.10	133.0
147.90	105.0
150.10	159.0
155.00	133.0
156.90	106.0
171.00	421.0
171.90	335.0
173.00	1005.0
174.00	54232.0
175.00	4112.0
176.00	51760.0
177.10	3044.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240

m/z	Abundance
35.90	481.0
37.00	2291.0
38.10	2275.0
39.10	1242.0
40.10	286.0
40.50	330.0
44.10	1100.0
45.00	367.0
46.10	236.0
47.10	868.0
48.10	447.0
49.00	2359.0
50.00	10796.0
51.00	3200.0
52.00	224.0
53.80	170.0
55.10	217.0
56.10	911.0
57.10	1563.0
59.90	544.0
61.10	3175.0
62.00	3074.0
63.00	2912.0
64.00	837.0
65.10	431.0
66.90	229.0
68.00	6097.0
69.10	5871.0
70.20	342.0
71.80	334.0
73.00	2979.0
74.10	11102.0
75.10	31256.0
76.00	2693.0
76.90	675.0
77.80	247.0
79.00	3739.0
80.00	789.0
81.00	4637.0
82.00	561.0
87.10	2660.0
88.00	3080.0
90.90	264.0
92.10	1984.0
93.00	2843.0
94.00	7661.0
95.10	66776.0
96.00	4000.0
97.10	139.0
104.00	430.0
104.80	118.0
105.90	513.0
106.80	112.0
108.00	198.0
109.80	113.0
114.90	103.0
115.90	277.0
116.90	633.0
117.90	276.0
119.00	671.0
128.10	255.0
129.00	226.0
129.80	294.0
131.00	110.0
134.80	140.0
137.10	192.0
140.90	644.0
142.10	109.0
143.00	1516.0
145.00	814.0
146.00	175.0
147.90	100.0
150.10	106.0
155.00	121.0
171.00	352.0
172.10	361.0
173.00	972.0
174.00	53976.0
175.00	4086.0
176.00	50880.0
177.00	2817.0

Instrument :
MSVOA_V
ClientSampleId :
BFB240