

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082118\
 Data File : VV007114.D
 Acq On : 21 Aug 2018 21:03
 Operator : SY/MD
 Sample : J4557-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J63

Quant Time: Aug 22 04:17:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 22 03:46:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	285666	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	278553	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	107844	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	100089	5.01	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.20%
7) Chloroethane-d5	1.58	69	83811	5.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.40%
11) 1,1-Dichloroethene-d2	2.13	63	135077	3.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.40%
20) 2-Butanone-d5	3.97	46	274578	59.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.30%
24) Chloroform-d	4.40	84	203231	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
26) 1,2-Dichloroethane-d4	5.09	65	105119	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.20%
32) Benzene-d6	5.10	84	394622	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	131060	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.37	98	301082	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
43) trans-1,3-Dichloropropene-	7.67	79	41096	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.15	63	112356	42.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.00%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	98200	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	107389	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	7521	2.82 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082118\
Data File : VV007114.D
Acq On : 21 Aug 2018 21:03
Operator : SY/MD
Sample : J4557-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J63

Quant Time: Aug 22 04:17:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 22 03:46:37 2018
Response via : Initial Calibration

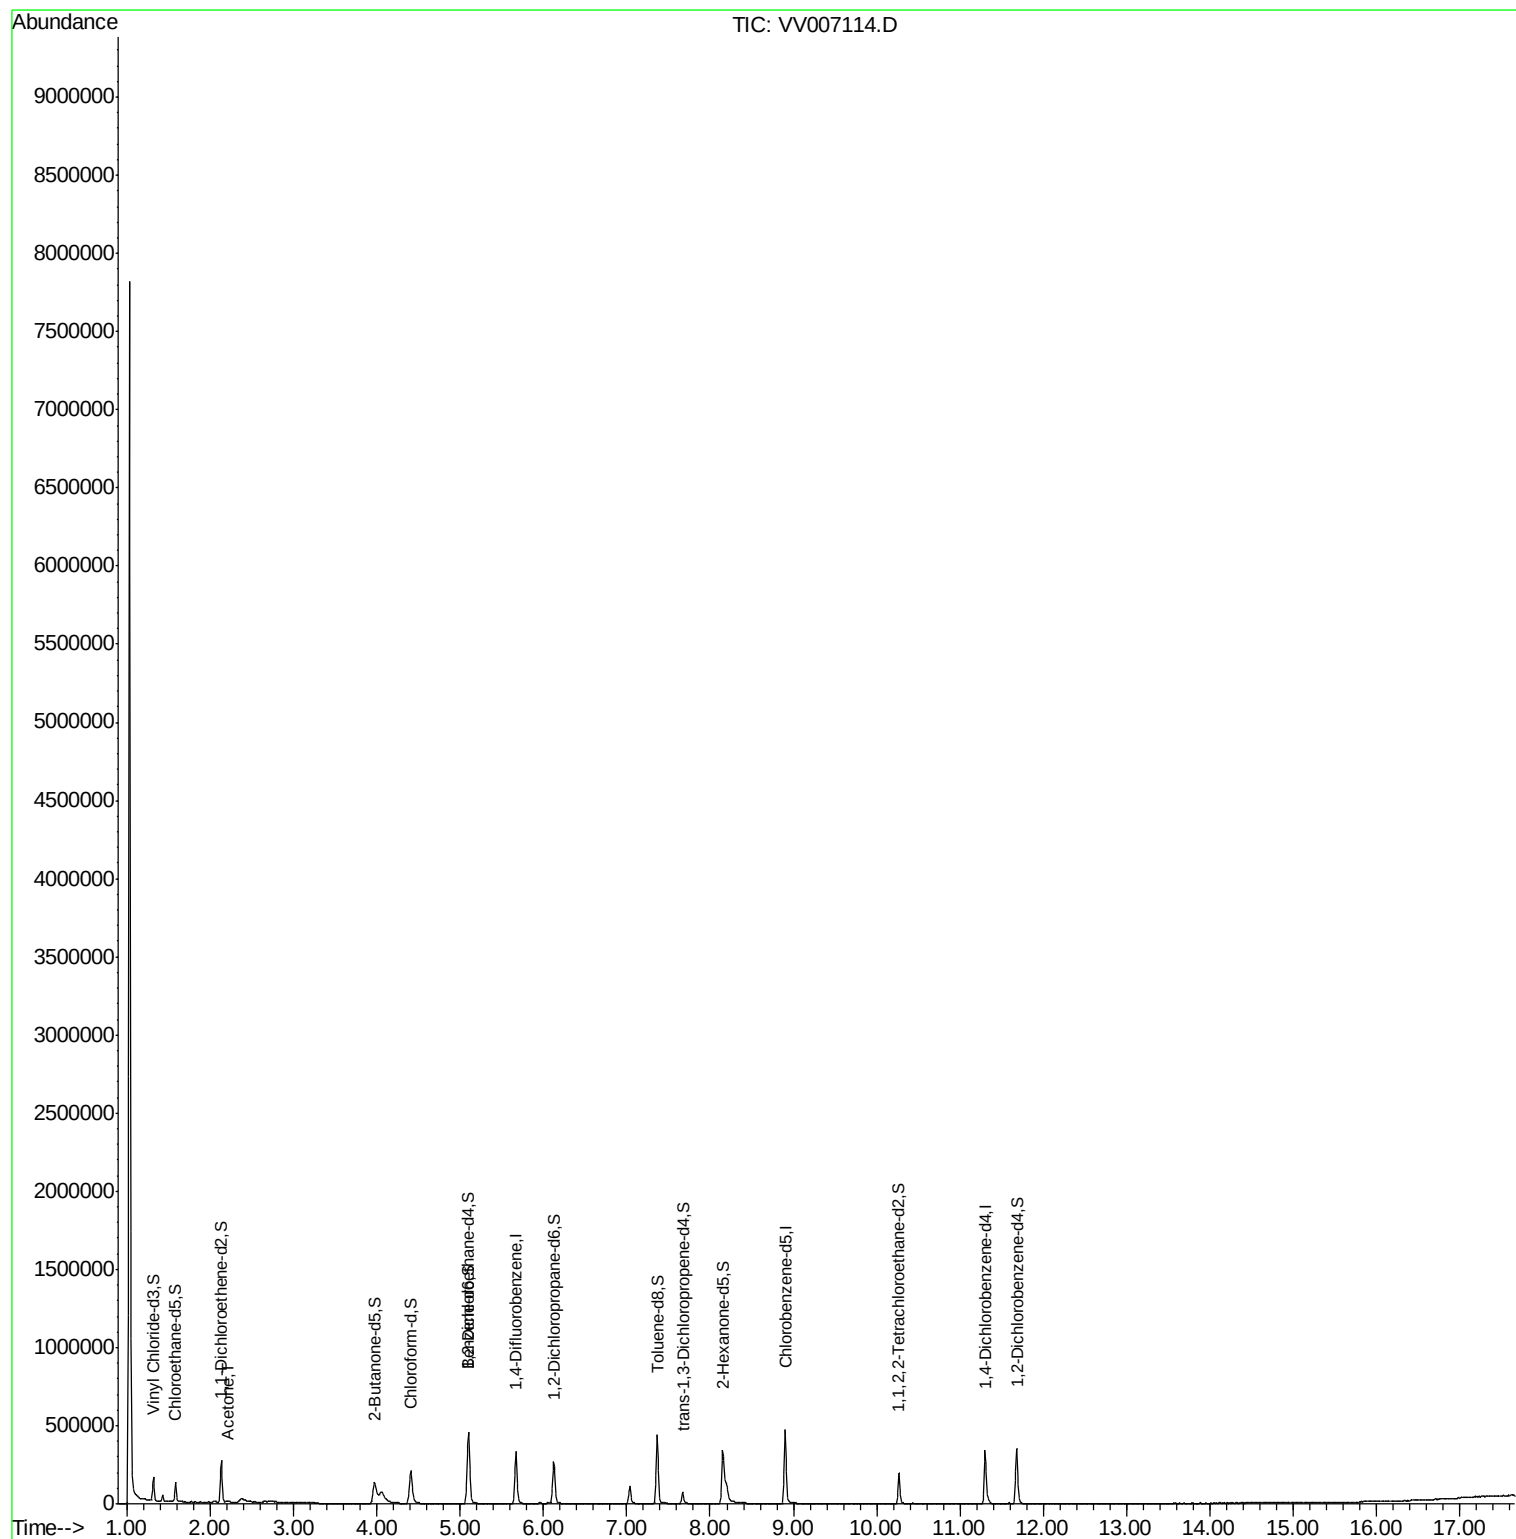

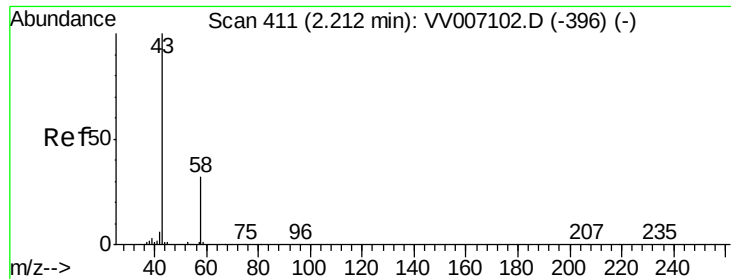

#13

Acetone

Concen: 2.82 ug/L

RT: 2.21 min Scan# 410

Delta R.T. -0.00 min

Lab File: VV007114.D

Acq: 21 Aug 2018 21:03

Instrument :
MSVOA_V
ClientSampleId :
C0J63

Tot Ion: 43 Resp: 7521

Ion Ratio Lower Upper

43 100

58 43.5 0.0 82.2

