

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082118\
 Data File : VV007115.D
 Acq On : 21 Aug 2018 21:29
 Operator : SY/MD
 Sample : J4557-02
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J64

Quant Time: Aug 22 04:18:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 22 03:46:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	270824	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	263770	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	99829	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	95068	5.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.40%
7) Chloroethane-d5	1.58	69	81927	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.80%
11) 1,1-Dichloroethene-d2	2.13	63	129488	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.98	46	277144	62.97	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.94%
24) Chloroform-d	4.40	84	193999	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.09	65	103984	5.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.80%
32) Benzene-d6	5.10	84	378299	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.12	67	128654	5.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.60%
41) Toluene-d8	7.37	98	281533	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
43) trans-1,3-Dichloropropene-	7.67	79	39818	4.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.60%
46) 2-Hexanone-d5	8.15	63	110273	44.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.10%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	96575	5.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	102576	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	6399	2.53 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082118\
Data File : VV007115.D
Acq On : 21 Aug 2018 21:29
Operator : SY/MD
Sample : J4557-02
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J64

Quant Time: Aug 22 04:18:06 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 22 03:46:37 2018
Response via : Initial Calibration

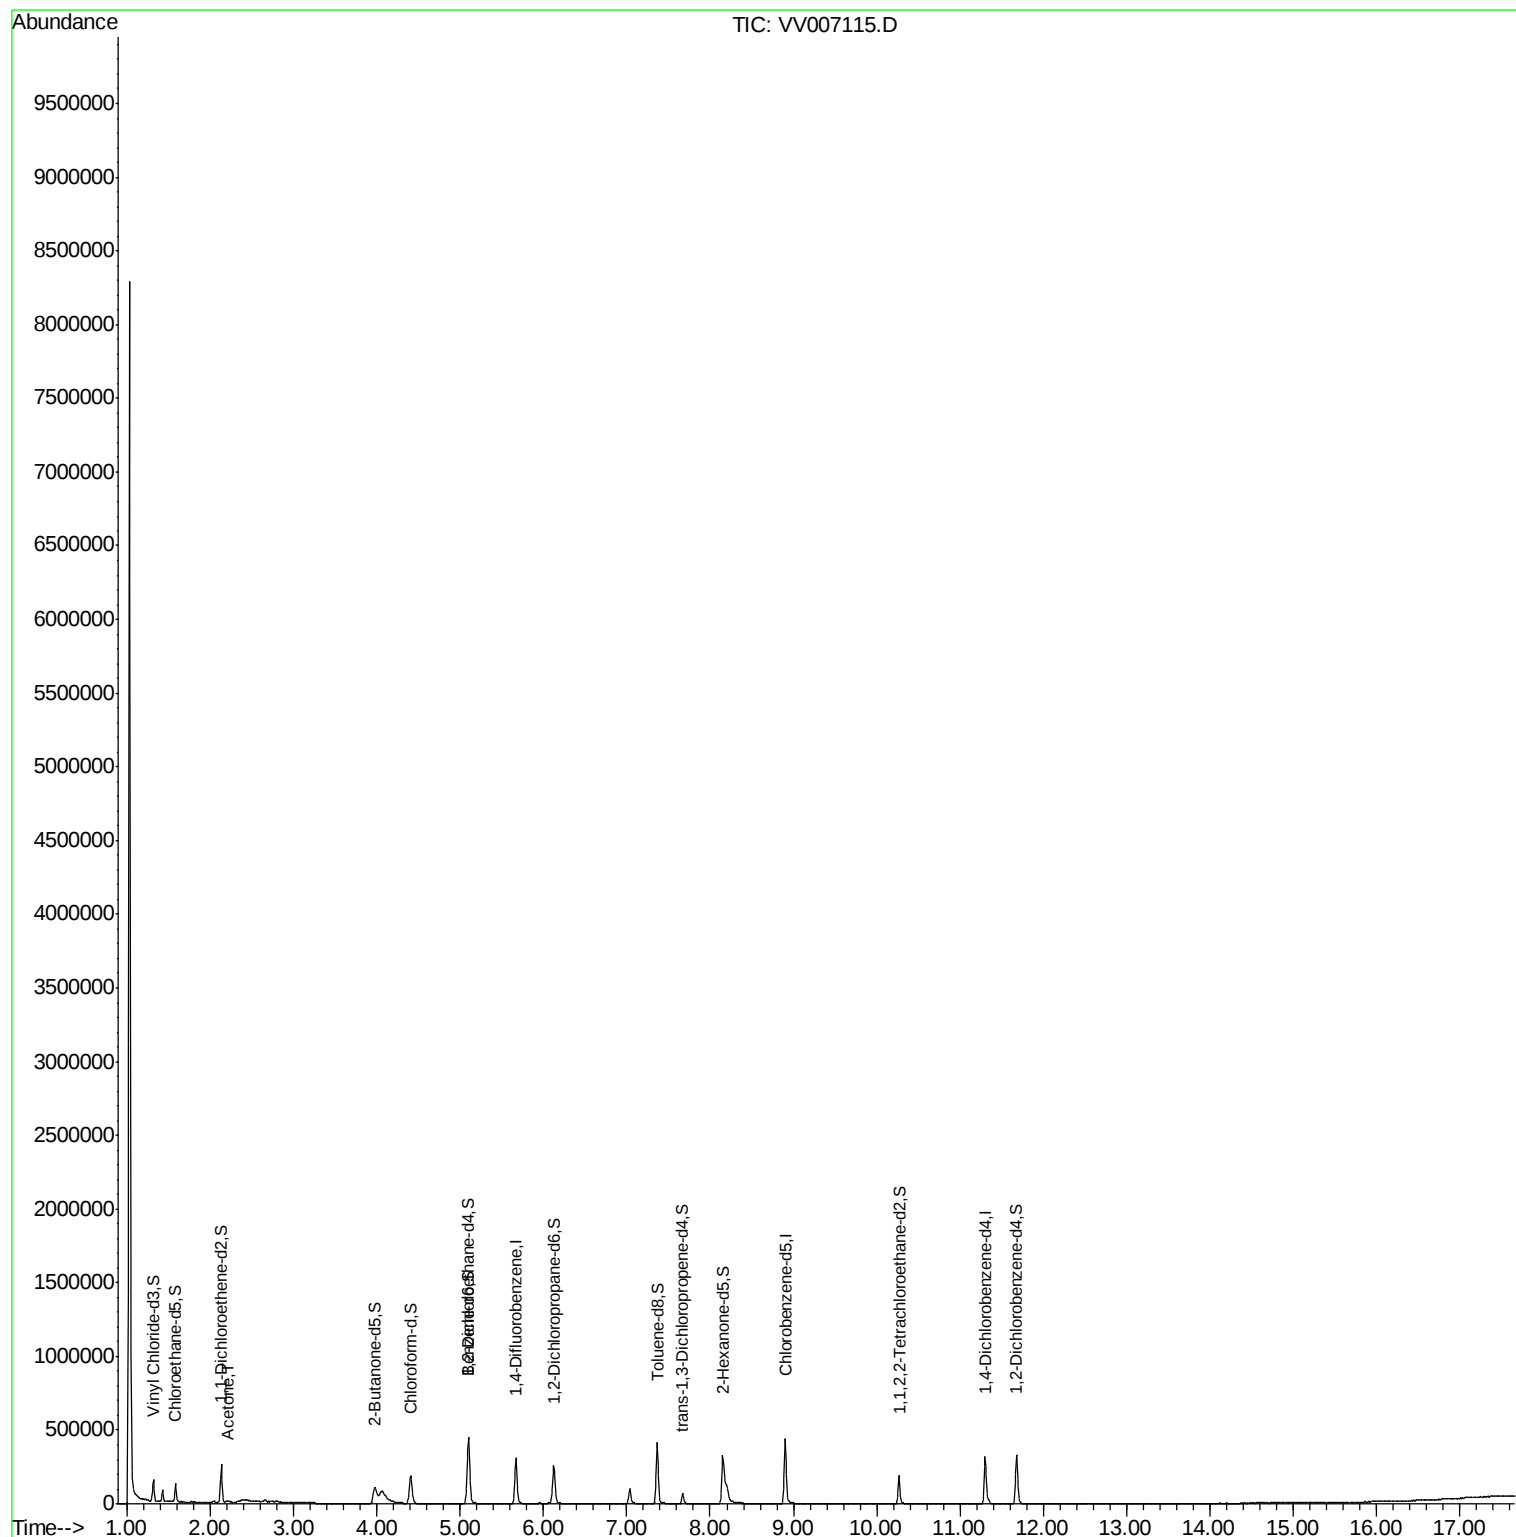

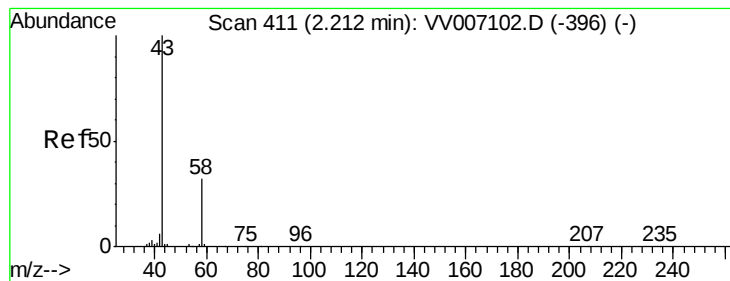

#13

Acetone

Concen: 2.53 ug/L

RT: 2.21 min Scan# 411

Delta R.T. 0.00 min

Lab File: VV007115.D

Acq: 21 Aug 2018 21:29

Instrument :
MSVOA_V
ClientSampleId :
C0J64

Tot Ion: 43 Resp: 6399

Ion Ratio Lower Upper

43 100

58 41.5 0.0 82.2

