

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082118\
 Data File : VV007116.D
 Acq On : 21 Aug 2018 21:56
 Operator : SY/MD
 Sample : J4557-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J65

Quant Time: Aug 22 04:19:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 22 03:46:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	278541	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	278850	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	107560	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96575	4.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.20%
7) Chloroethane-d5	1.58	69	80827	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.13	63	131104	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	3.97	46	274229	60.59	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.18%
24) Chloroform-d	4.41	84	198092	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
26) 1,2-Dichloroethane-d4	5.09	65	101250	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.80%
32) Benzene-d6	5.10	84	376910	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.12	67	127619	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.37	98	286594	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.20%
43) trans-1,3-Dichloropropene-	7.67	79	40378	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.15	63	110294	41.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.36%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	94682	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	105766	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	15527	5.97 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082118\
Data File : VV007116.D
Acq On : 21 Aug 2018 21:56
Operator : SY/MD
Sample : J4557-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J65

Quant Time: Aug 22 04:19:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 22 03:46:37 2018
Response via : Initial Calibration

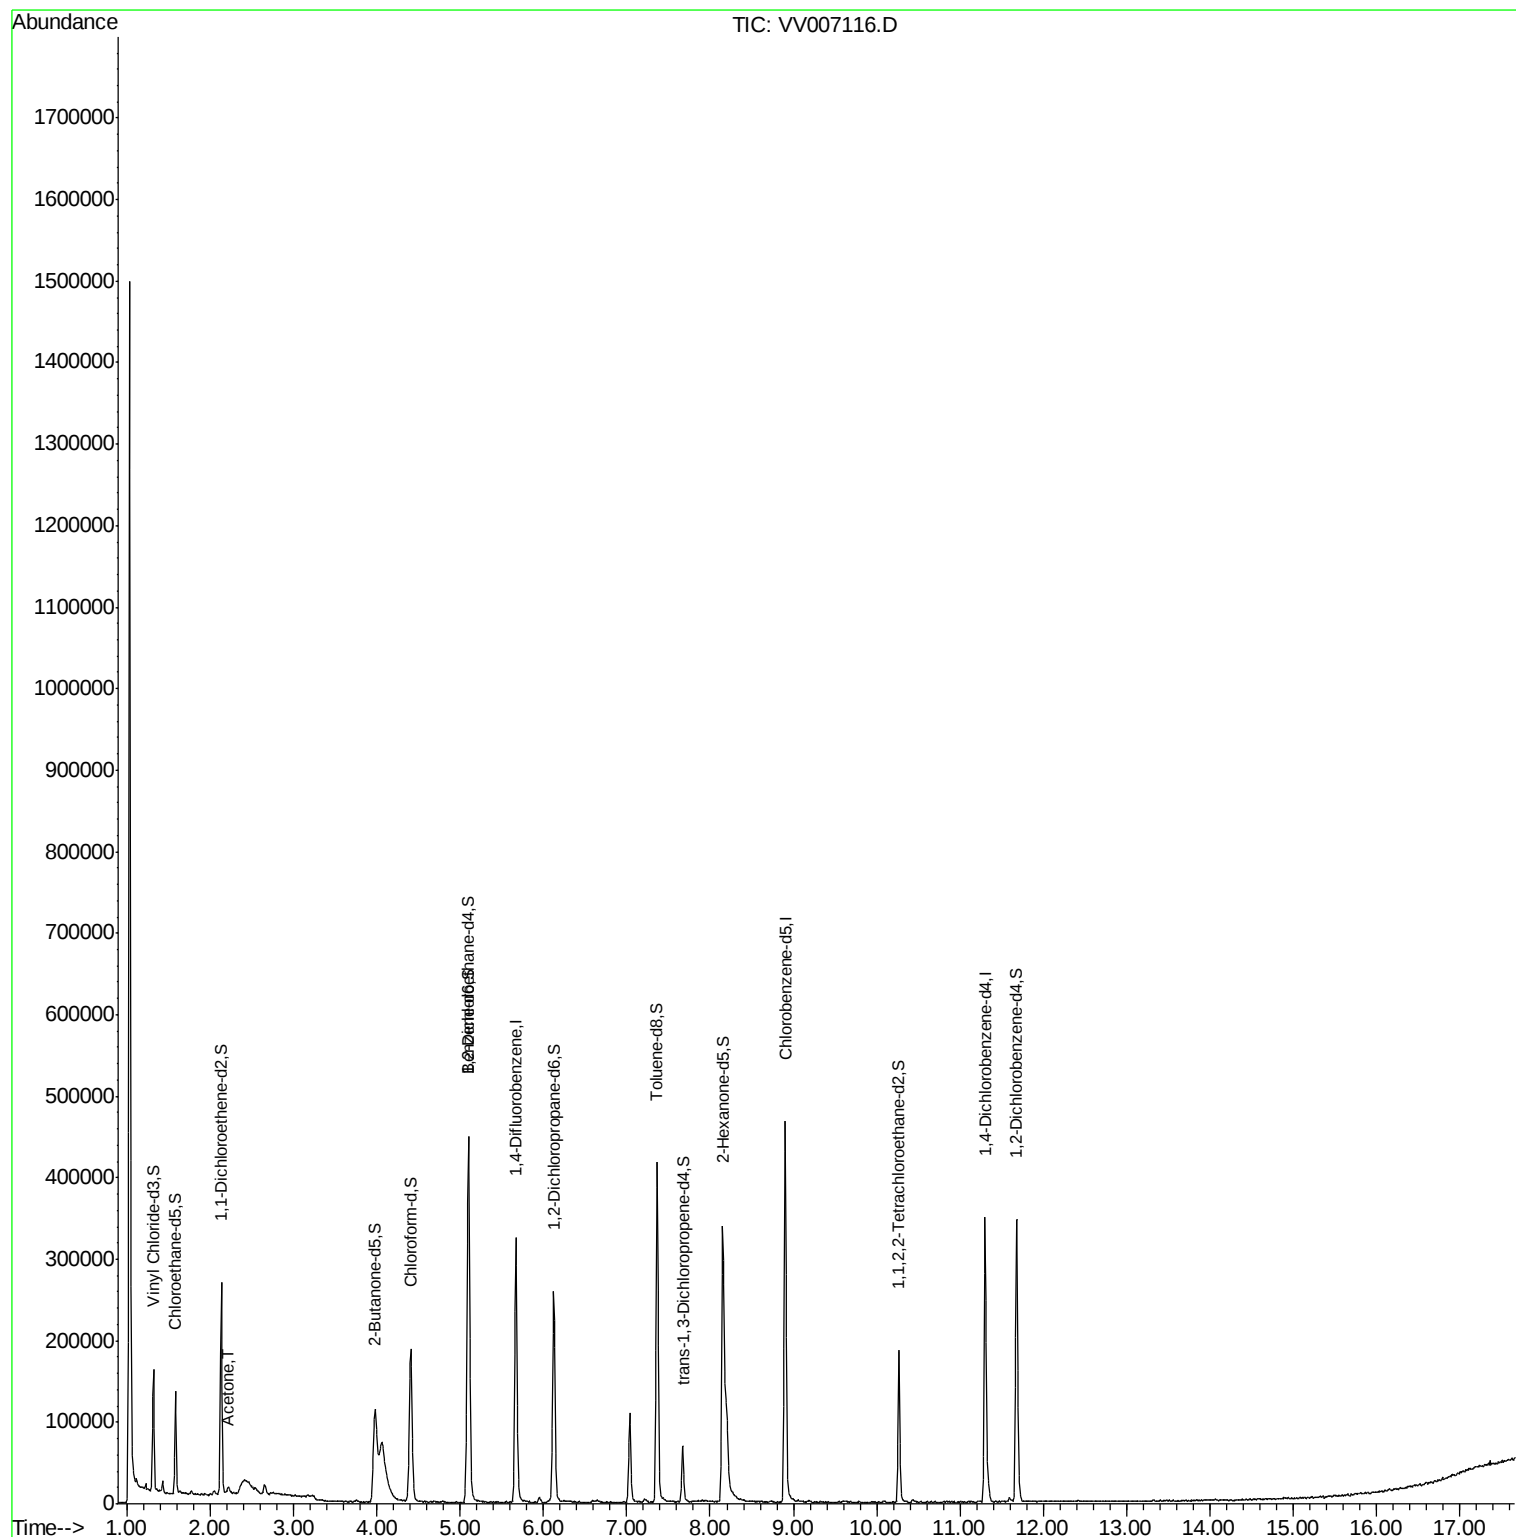

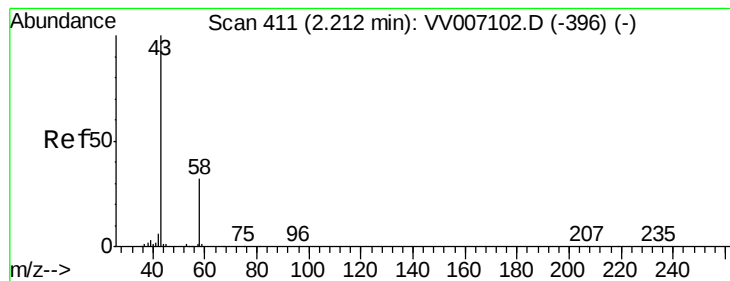

#13

Acetone

Concen: 5.97 ug/L

RT: 2.21 min Scan# 411

Delta R.T. 0.00 min

Lab File: VV007116.D

Acq: 21 Aug 2018 21:56

Instrument :
MSVOA_V
ClientSampleId :
C0J65

Tot Ion: 43 Resp: 15527

Ion Ratio Lower Upper

43 100

58 30.4 0.0 82.2

