


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082118\
 Data File : VV007098.D
 Acq On : 21 Aug 2018 11:56
 Operator : SY/MD
 Sample : BFB61
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB61

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 22 03:46:37 2018

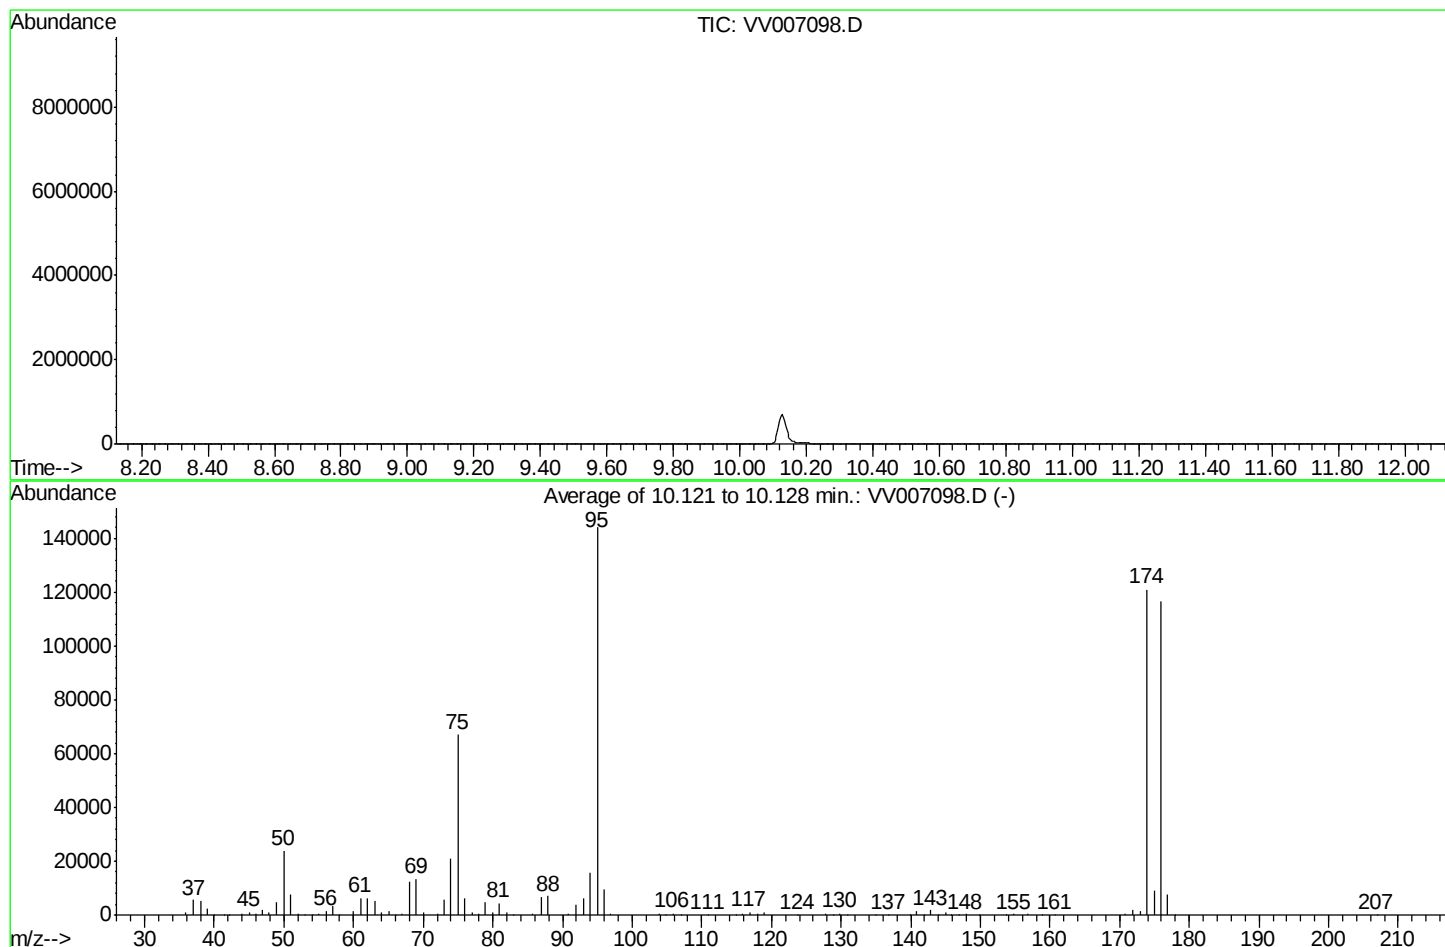

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	23877	PASS
75	95	30	80	46.5	67002	PASS
95	95	100	100	100.0	144106	PASS
96	95	5	9	6.5	9334	PASS
173	174	0.00	2	1.1	1313	PASS
174	95	50	120	83.9	120901	PASS
175	174	5	9	7.5	9113	PASS
176	174	95	101	96.3	116376	PASS
177	176	5	9	6.5	7514	PASS

Scan 2858 (10.080 min): VV007098.D
BFB61

m/z	Abundance
39.90	463.0
43.90	1356.0
206.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.00	977.0
37.00	5401.0
38.00	4836.0
39.10	2076.0
40.00	601.0
41.30	128.0
43.90	1661.0
45.00	1006.0
45.90	296.0
46.90	2150.0
47.90	752.0
49.00	4703.0
50.00	22640.0
51.00	7260.0
51.90	360.0
52.90	219.0
55.00	313.0
56.00	1472.0
57.00	3118.0
57.90	133.0
60.00	1276.0
61.00	6442.0
62.00	5934.0
63.00	4996.0
64.00	1125.0
65.00	1644.0
66.00	141.0
67.00	390.0
68.00	12028.0
69.00	12575.0
70.00	857.0
72.00	643.0
73.00	5317.0
74.00	20024.0
75.00	63616.0
76.00	5995.0
77.00	883.0
77.90	604.0
78.90	4369.0
79.90	1105.0
80.90	4075.0
81.90	692.0
83.00	127.0
85.80	279.0
86.90	6096.0
87.90	6478.0
90.80	437.0
92.00	3525.0
93.00	5493.0
94.00	14923.0
95.00	136576.0
96.00	8594.0
96.90	200.0
103.90	538.0
104.80	133.0
105.80	530.0
107.00	171.0
110.80	103.0
114.90	141.0
115.80	461.0
116.90	875.0
118.00	464.0
118.90	828.0
123.80	137.0
127.80	406.0
128.80	186.0
129.80	499.0
130.80	118.0
135.00	162.0
136.90	222.0
140.80	1159.0
142.00	231.0
142.80	1694.0
144.00	141.0
145.00	649.0
145.90	247.0
146.80	136.0
147.90	282.0
149.90	114.0
154.90	440.0
156.90	247.0
160.70	117.0
170.80	396.0
171.90	1638.0
173.00	1332.0
173.90	110784.0
174.90	8449.0
175.90	108168.0
176.90	7053.0
177.90	133.0
206.90	280.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
35.90	948.0
37.00	5880.0
38.00	5261.0
39.00	2226.0
40.00	562.0
41.30	172.0
42.20	115.0
43.90	1806.0
45.00	1020.0
45.90	340.0
46.90	2126.0
47.90	764.0
49.00	5044.0
50.00	24712.0
51.00	7724.0
52.00	424.0
52.90	233.0
54.00	144.0
55.00	325.0
56.00	1559.0
57.00	3234.0
60.00	1416.0
61.00	6351.0
62.00	6282.0
63.00	5323.0
64.00	1108.0
65.00	1735.0
66.00	168.0
67.00	523.0
68.00	12974.0
69.00	13994.0
70.00	1011.0
72.00	675.0
73.00	6054.0
74.00	21504.0
75.00	68736.0
76.00	6302.0
77.00	973.0
77.90	661.0
78.90	4708.0
79.90	1252.0
80.90	4549.0
82.00	879.0
83.00	169.0
85.70	329.0
86.90	6754.0
87.90	7391.0
90.80	441.0
92.00	3697.0
93.00	6269.0
94.00	16336.0
95.00	148864.0
96.00	9612.0
96.90	277.0
103.90	519.0
104.80	145.0
105.90	605.0
107.00	187.0
110.90	128.0
114.90	169.0
115.90	466.0
116.90	976.0
117.90	521.0
118.80	870.0
123.80	186.0
127.80	437.0
128.90	204.0
129.80	492.0
130.80	139.0
135.00	147.0
136.80	247.0
139.80	108.0
140.80	1312.0
142.00	244.0
142.90	1950.0
143.90	121.0
145.00	796.0
145.80	189.0
146.80	125.0
148.00	325.0
149.90	144.0
154.80	381.0
156.80	319.0
158.80	174.0
160.70	145.0
170.90	438.0
171.90	1874.0
173.00	1339.0
173.90	124040.0
174.90	9434.0
175.90	119936.0
176.90	7747.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

177.90116.0

207.00309.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	900.0
37.00	5760.0
38.00	5314.0
39.00	2423.0
40.00	565.0
41.30	118.0
43.90	1880.0
45.00	1003.0
45.90	332.0
46.90	1977.0
47.90	747.0
49.00	4850.0
50.00	24280.0
51.00	7403.0
52.00	442.0
52.90	257.0
54.00	179.0
55.00	348.0
56.00	1642.0
57.00	3056.0
59.90	1341.0
61.00	5795.0
62.00	6178.0
63.00	5080.0
64.00	1046.0
65.00	1649.0
66.00	195.0
66.90	523.0
68.00	12605.0
69.00	14134.0
70.00	1136.0
72.00	661.0
73.00	6191.0
74.00	21520.0
75.00	68656.0
76.00	6210.0
77.00	1046.0
77.90	634.0
78.90	4606.0
79.90	1266.0
80.90	4597.0
82.00	1116.0
83.00	220.0
85.70	396.0
86.90	6866.0
87.90	7290.0
90.90	387.0
92.00	3693.0
93.00	6361.0
94.00	16045.0
95.00	146880.0
96.00	9797.0
96.90	302.0
103.90	467.0
104.80	133.0
105.90	636.0
106.80	150.0
111.00	125.0
114.90	149.0
115.90	423.0
116.90	1014.0
117.90	514.0
118.80	886.0
123.80	167.0
127.80	421.0
128.90	190.0
129.80	451.0
130.90	138.0
134.90	138.0
136.80	236.0
139.80	156.0
140.80	1301.0
141.90	199.0
142.90	1994.0
143.80	102.0
145.00	890.0
145.80	143.0
148.00	323.0
149.90	170.0
153.70	124.0
154.80	332.0
156.80	370.0
158.90	275.0
160.70	150.0
170.90	392.0
172.00	2047.0
173.00	1269.0
173.90	127880.0
175.00	9458.0
175.90	121024.0
176.90	7742.0
177.90	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

207.00

320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61