

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012327.D
 Acq On : 21 Aug 2019 21:09
 Operator : SY/MD
 Sample : K4464-04
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW1

Quant Time: Aug 22 04:19:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 22 03:48:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	219639	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	206296	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	95413	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48130	46.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.56%
7) Chloroethane-d5	1.58	69	36943	49.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.10%
11) 1,1-Dichloroethene-d2	2.13	63	76821	37.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.06%
21) 2-Butanone-d5	3.93	46	68838	84.93	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.93%
24) Chloroform-d	4.40	84	139616	47.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.48%
26) 1,2-Dichloroethane-d4	5.08	65	104582	51.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.62%
32) Benzene-d6	5.10	84	272005	49.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.88%
36) 1,2-Dichloropropane-d6	6.12	67	73491	49.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.80%
41) Toluene-d8	7.36	98	262504	48.96	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.92%
43) trans-1,3-Dichloropropene-	7.66	79	42768	46.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.36%
47) 2-Hexanone-d5	8.13	63	57384	93.46	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.46%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	102404	48.33	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.66%
64) 1,2-Dichlorobenzene-d4	11.67	152	109232	52.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.16%


Target Compounds					Ovalue
13) Acetone	2.19	43	2674	4.396 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012327.D
Acq On : 21 Aug 2019 21:09
Operator : SY/MD
Sample : K4464-04
Misc : 5mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW1

Quant Time: Aug 22 04:19:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 22 03:48:59 2019
Response via : Initial Calibration

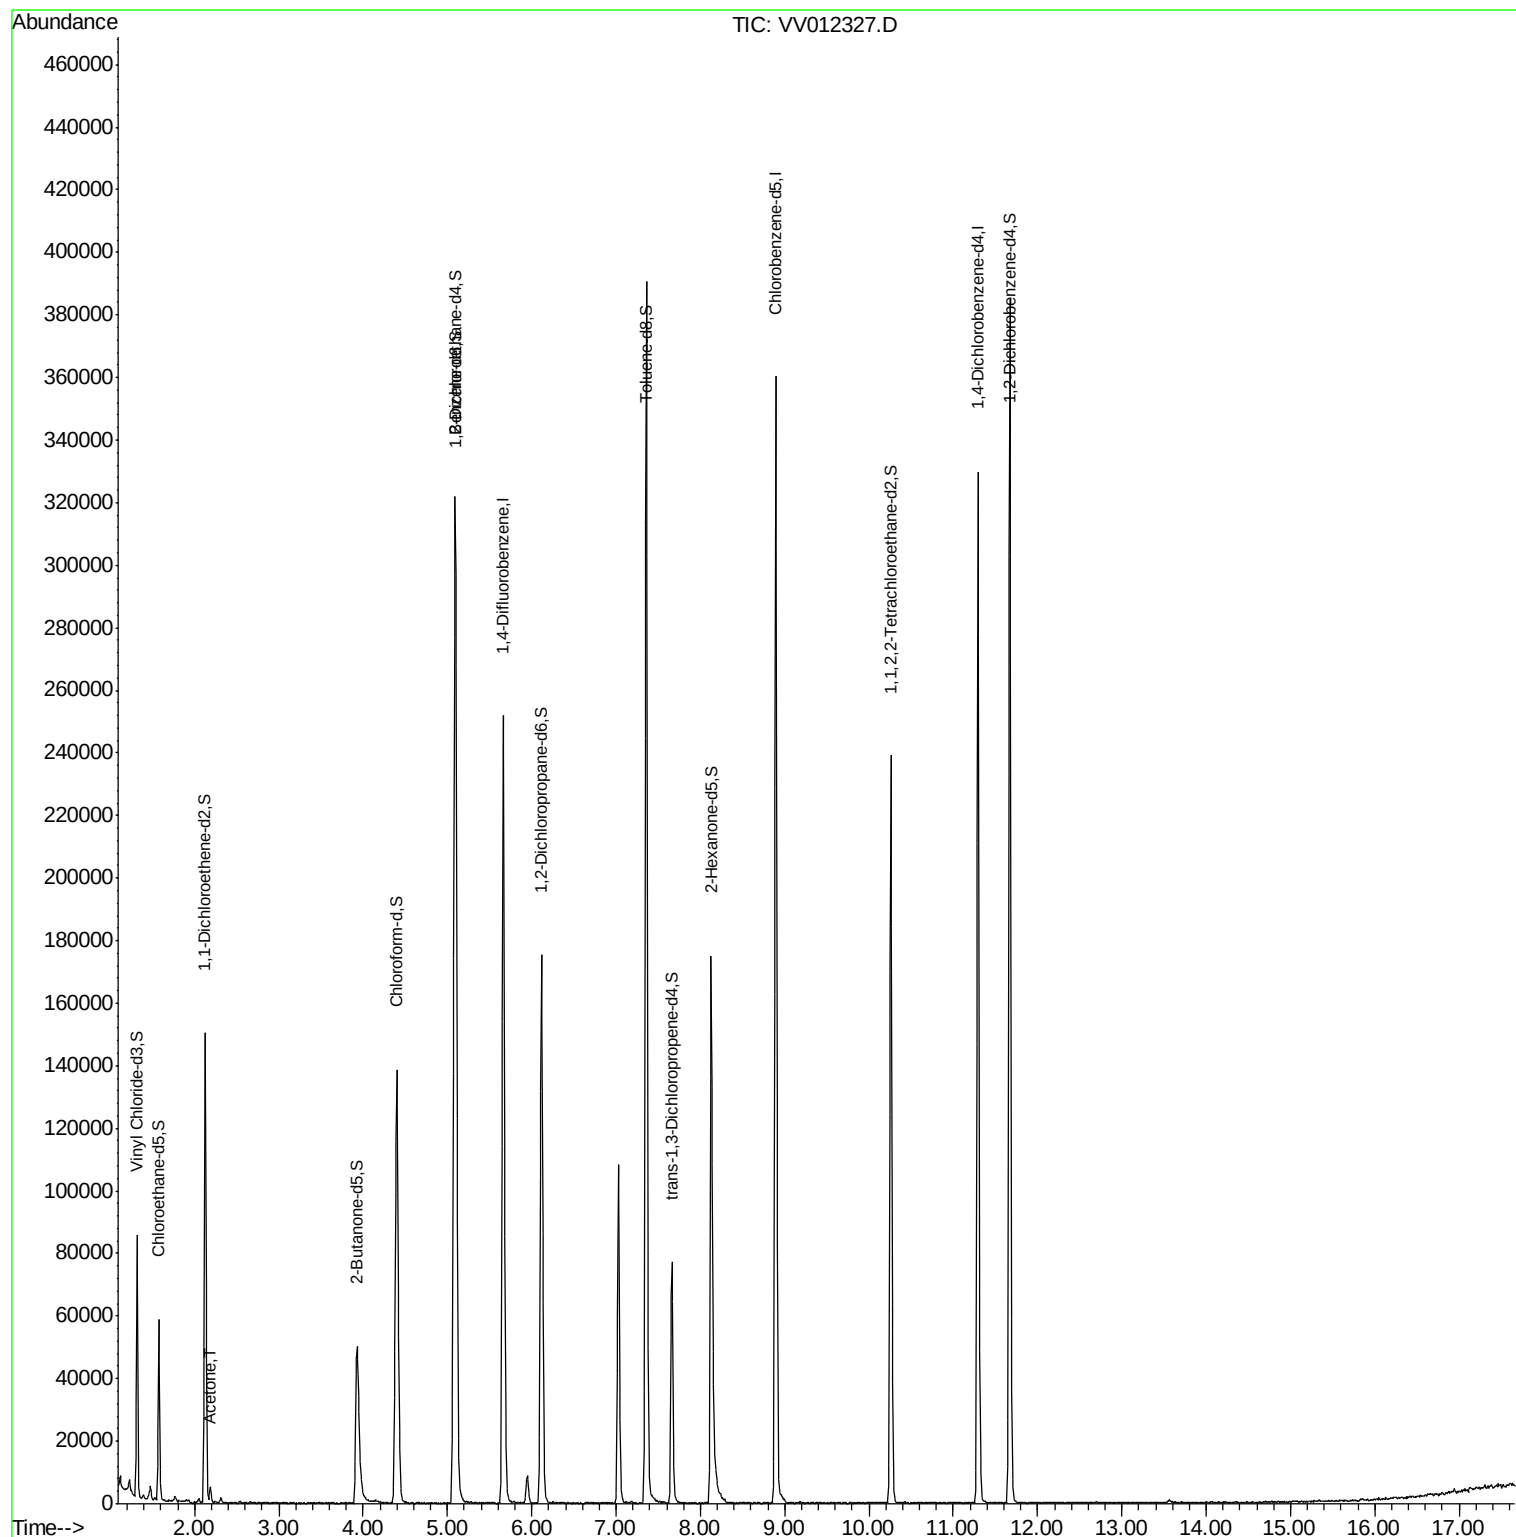

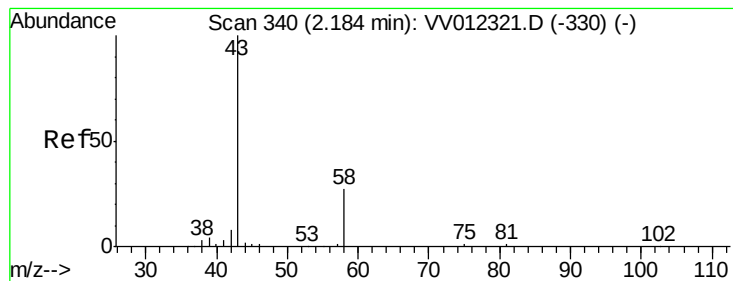

#13

Acetone

Concen: 4.396 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV012327.D

Acq: 21 Aug 2019 21:09

Instrument :
MSVOA_V
ClientSampleId :
BEJW1

Tot Ion: 43 Resp: 2674

Ion Ratio Lower Upper

43 100

58 24.3 0.0 54.2

