

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012325.D
 Acq On : 21 Aug 2019 20:21
 Operator : SY/MD
 Sample : K4464-02
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJT9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	83	rVB	79115	81659	10.27%	1.356%
2	1.579	145	152	167	rVB	58325	67623	8.50%	1.123%
3	2.055	294	300	302	rBV3	1217	1308	0.16%	0.022%
4	2.129	312	323	334	rBV	150410	210060	26.41%	3.489%
5	2.447	417	422	425	rBV2	335	403	0.05%	0.007%
6	2.502	436	439	442	rBV2	329	264	0.03%	0.004%
7	2.592	464	467	469	rBB	208	92	0.01%	0.002%
8	2.605	469	471	473	rBV	228	126	0.02%	0.002%
9	2.804	531	533	534	rBV	128	51	0.01%	0.001%
10	2.868	549	553	558	rBV	299	321	0.04%	0.005%
11	2.891	558	560	566	rVB2	304	201	0.03%	0.003%
12	2.917	566	568	569	rBV	262	122	0.02%	0.002%
13	3.100	621	625	629	rBV2	463	336	0.04%	0.006%
14	3.190	651	653	659	rVB2	194	148	0.02%	0.002%
15	3.222	660	663	669	rVB	224	194	0.02%	0.003%
16	3.248	669	671	673	rBV	155	55	0.01%	0.001%
17	3.312	689	691	696	rVB2	241	179	0.02%	0.003%
18	3.338	696	699	706	rVB2	274	338	0.04%	0.006%
19	3.392	713	716	719	rBV2	219	172	0.02%	0.003%
20	3.560	765	768	772	rVB	188	156	0.02%	0.003%
21	3.685	805	807	811	rBV	163	128	0.02%	0.002%
22	3.772	827	834	837	rBV2	474	657	0.08%	0.011%
23	3.810	845	846	849	rBV2	119	63	0.01%	0.001%
24	3.839	852	855	859	rBV	188	152	0.02%	0.003%
25	3.859	859	861	863	rBV	150	46	0.01%	0.001%
26	3.926	870	882	919	rBV2	50794	149456	18.79%	2.482%
27	4.399	1013	1029	1059	rVB	136400	331776	41.71%	5.511%
28	4.563	1078	1080	1083	rBV2	252	135	0.02%	0.002%
29	4.611	1093	1095	1096	rBV	155	42	0.01%	0.001%
30	4.637	1101	1103	1107	rBV	176	129	0.02%	0.002%
31	4.659	1108	1110	1112	rVB	165	66	0.01%	0.001%
32	4.707	1119	1125	1127	rBV2	284	234	0.03%	0.004%
33	4.807	1153	1156	1159	rVB2	244	179	0.02%	0.003%
34	5.093	1225	1245	1275	rBV2	315599	795349	100.00%	13.210%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012325.D
 Acq On : 21 Aug 2019 20:21
 Operator : SY/MD
 Sample : K4464-02
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJT9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	5.402	1338	1341	1343	rBV2	150	94	0.01%	0.002%
36	5.492	1367	1369	1372	rBV	267	122	0.02%	0.002%
37	5.662	1407	1422	1448	rBV	262084	512854	64.48%	8.518%
38	5.949	1500	1511	1524	rVB3	8366	16096	2.02%	0.267%
39	6.116	1549	1563	1581	rBV	171343	342605	43.08%	5.690%
40	6.283	1611	1615	1618	rVB3	408	299	0.04%	0.005%
41	6.312	1621	1624	1627	rBV	235	195	0.02%	0.003%
42	6.421	1654	1658	1661	rBV	265	207	0.03%	0.003%
43	6.534	1690	1693	1696	rBV	223	130	0.02%	0.002%
44	6.640	1723	1726	1727	rBV	184	81	0.01%	0.001%
45	6.650	1727	1729	1734	rVB2	433	295	0.04%	0.005%
46	6.826	1783	1784	1786	rBV	124	42	0.01%	0.001%
47	6.916	1810	1812	1813	rBV	195	70	0.01%	0.001%
48	6.952	1821	1823	1827	rBV	142	90	0.01%	0.001%
49	7.029	1834	1847	1873	rBV	106903	191206	24.04%	3.176%
50	7.180	1891	1894	1898	rVB2	311	232	0.03%	0.004%
51	7.235	1909	1911	1914	rBV	270	131	0.02%	0.002%
52	7.357	1936	1949	1968	rBV	392143	677722	85.21%	11.257%
53	7.617	2027	2030	2033	rBV	188	114	0.01%	0.002%
54	7.662	2033	2044	2064	rBV	77280	128433	16.15%	2.133%
55	8.129	2178	2189	2222	rBV2	168096	334486	42.06%	5.556%
56	8.466	2291	2294	2297	rBV2	203	176	0.02%	0.003%
57	8.576	2326	2328	2331	rBV2	262	142	0.02%	0.002%
58	8.794	2394	2396	2397	rBV2	184	82	0.01%	0.001%
59	8.894	2415	2427	2453	rBV	378156	613257	77.11%	10.186%
60	9.080	2482	2485	2489	rBV	351	302	0.04%	0.005%
61	9.177	2511	2515	2523	rBV2	682	952	0.12%	0.016%
62	9.267	2540	2543	2544	rBV	201	136	0.02%	0.002%
63	9.315	2556	2558	2560	rBV	160	86	0.01%	0.001%
64	9.395	2575	2583	2589	rBV2	235	457	0.06%	0.008%
65	9.775	2695	2701	2703	rBV	206	251	0.03%	0.004%
66	9.788	2704	2705	2706	rVB	130	30	0.00%	0.000%
67	9.942	2749	2753	2754	rBV	169	124	0.02%	0.002%
68	10.064	2789	2791	2793	rBV2	189	124	0.02%	0.002%
69	10.193	2825	2831	2836	rBV2	280	332	0.04%	0.006%
70	10.260	2839	2852	2871	rVV	236077	375935	47.27%	6.244%
71	10.772	3006	3011	3014	rBV2	308	353	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012325.D
 Acq On : 21 Aug 2019 20:21
 Operator : SY/MD
 Sample : K4464-02
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJT9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	10.926	3057	3059	3064	rBV	187	70	0.01%	0.001%
73	11.000	3078	3082	3087	rBV2	256	339	0.04%	0.006%
74	11.199	3141	3144	3146	rBV2	382	250	0.03%	0.004%
75	11.292	3161	3173	3195	rBV	350874	561159	70.56%	9.320%
76	11.524	3242	3245	3250	rBV2	240	289	0.04%	0.005%
77	11.669	3278	3290	3312	rBV	384301	617211	77.60%	10.251%
78	11.781	3324	3325	3331	rBV2	409	278	0.03%	0.005%
79	12.071	3410	3415	3417	rBV2	314	294	0.04%	0.005%
80	12.186	3450	3451	3452	rBV	256	53	0.01%	0.001%
81	13.794	3949	3951	3955	rBV2	428	306	0.04%	0.005%


Sum of corrected areas: 6020712

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012325.D
Acq On : 21 Aug 2019 20:21
Operator : SY/MD
Sample : K4464-02
Misc : 5mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJT9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

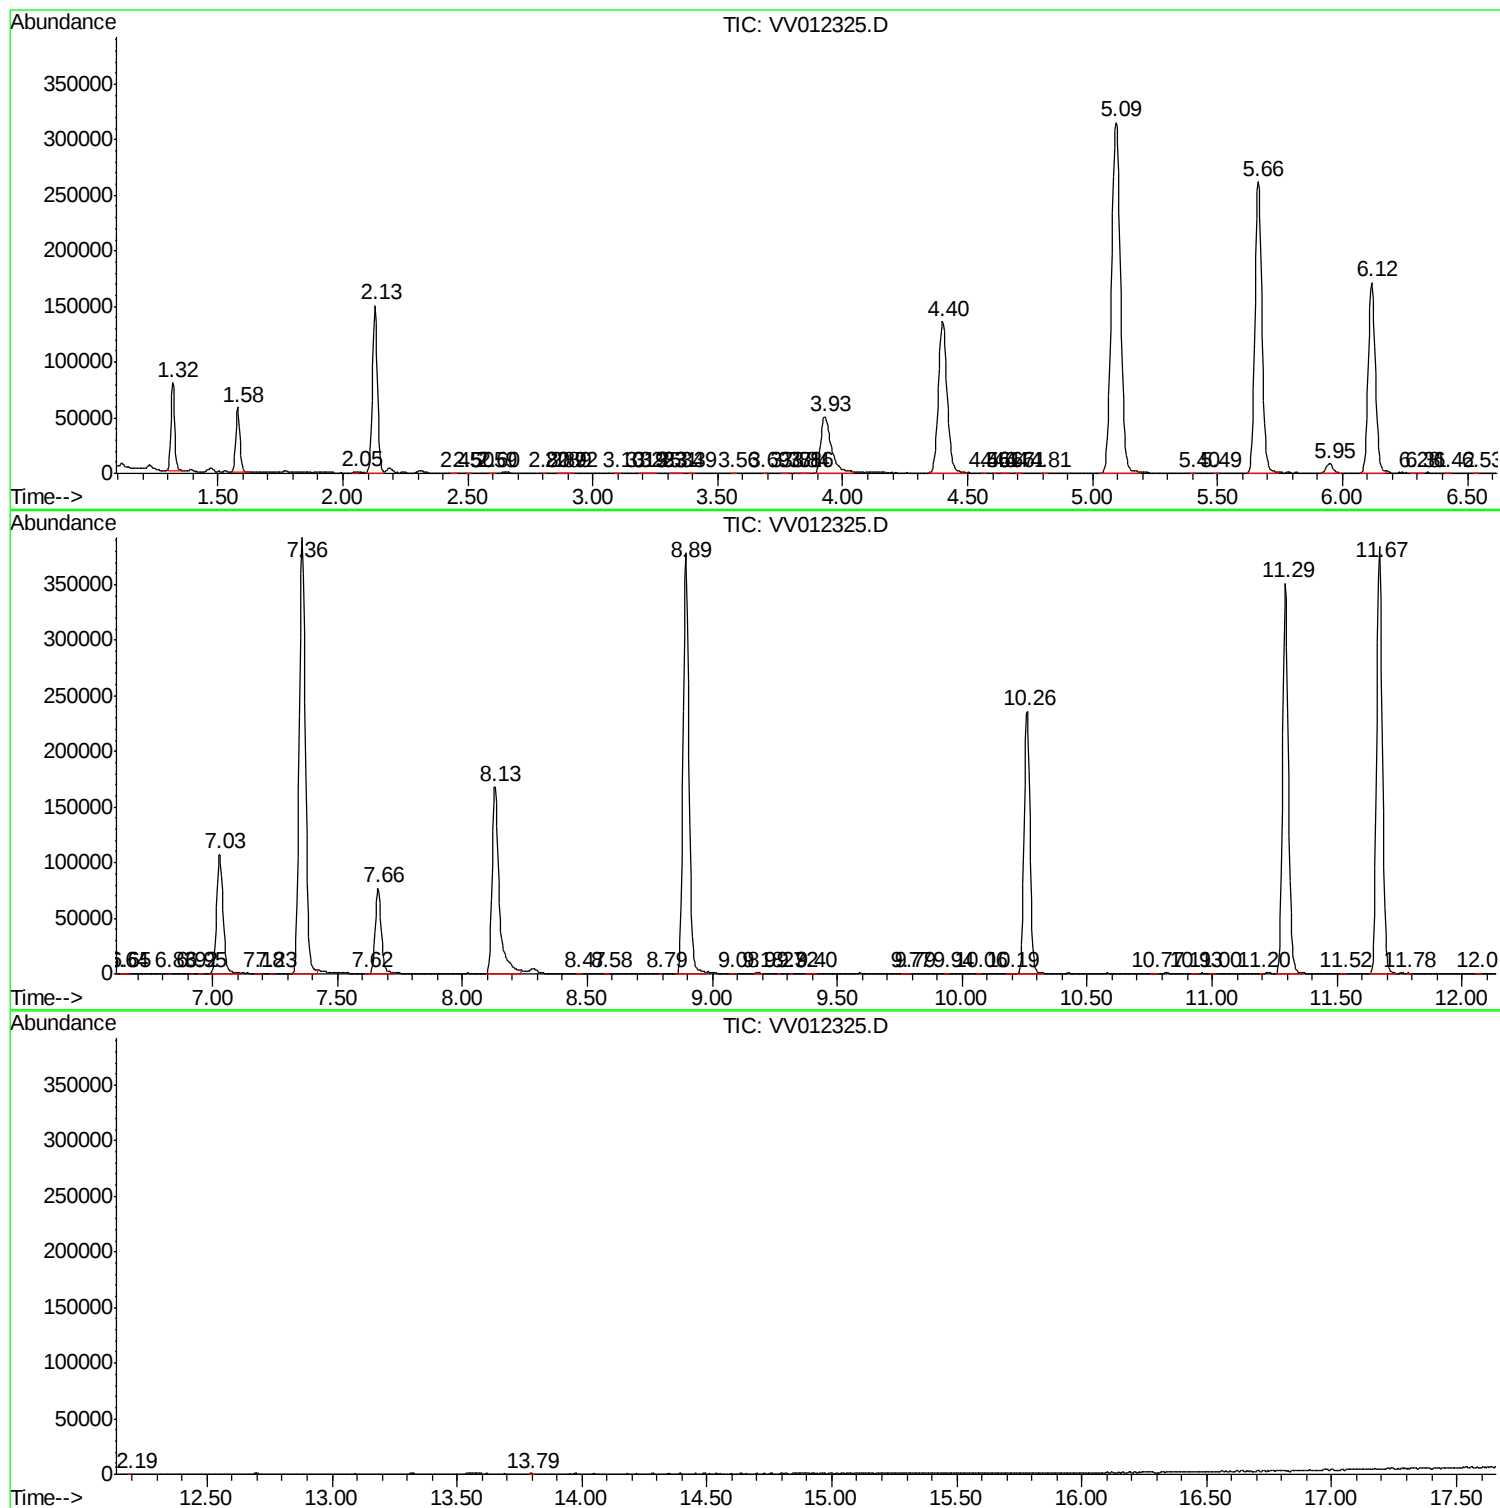

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082119\
Data File : VV012325.D
Acq On : 21 Aug 2019 20:21
Operator : SY/MD
Sample : K4464-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJT9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012325.D
Acq On : 21 Aug 2019 20:21
Operator : SY/MD
Sample : K4464-02
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEJT9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc