

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012326.D
 Acq On : 21 Aug 2019 20:45
 Operator : SY/MD
 Sample : K4464-03
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	86	rVB	80179	83060	10.34%	1.405%
2	1.579	144	152	166	rVB	57328	68137	8.48%	1.153%
3	2.026	287	291	293	rBV	551	373	0.05%	0.006%
4	2.129	313	323	335	rBV	147685	208762	25.99%	3.532%
5	2.540	450	451	453	rBV	208	98	0.01%	0.002%
6	2.589	463	466	469	rBV	165	144	0.02%	0.002%
7	2.759	518	519	520	rBV	235	75	0.01%	0.001%
8	2.798	528	531	532	rBV	310	216	0.03%	0.004%
9	3.010	593	597	602	rVB	237	263	0.03%	0.004%
10	3.042	602	607	610	rBV2	275	334	0.04%	0.006%
11	3.232	663	666	669	rBB2	166	101	0.01%	0.002%
12	3.293	683	685	687	rBV	167	49	0.01%	0.001%
13	3.370	707	709	713	rVB2	309	228	0.03%	0.004%
14	3.396	713	717	718	rBV	132	94	0.01%	0.002%
15	3.473	740	741	742	rBV	209	58	0.01%	0.001%
16	3.646	789	795	796	rBV	214	215	0.03%	0.004%
17	3.714	813	816	819	rVB2	187	135	0.02%	0.002%
18	3.740	821	824	827	rBV	198	134	0.02%	0.002%
19	3.814	846	847	849	rVB	124	46	0.01%	0.001%
20	3.868	861	864	867	rBV2	212	142	0.02%	0.002%
21	3.926	869	882	915	rBV2	45807	143448	17.86%	2.427%
22	4.212	968	971	977	rBV2	335	377	0.05%	0.006%
23	4.309	999	1001	1005	rBV	278	162	0.02%	0.003%
24	4.399	1011	1029	1058	rBV	134598	333630	41.54%	5.645%
25	4.653	1106	1108	1110	rBV	138	41	0.01%	0.001%
26	4.691	1117	1120	1123	rBV2	238	164	0.02%	0.003%
27	4.762	1139	1142	1147	rVB2	252	178	0.02%	0.003%
28	4.785	1147	1149	1152	rBV	191	93	0.01%	0.002%
29	4.798	1152	1153	1154	rBV	135	40	0.00%	0.001%
30	4.839	1164	1166	1170	rVB2	302	129	0.02%	0.002%
31	4.923	1190	1192	1197	rVB2	230	185	0.02%	0.003%
32	5.093	1226	1245	1275	rBV2	318125	803160	100.00%	13.588%
33	5.290	1304	1306	1309	rVB	282	149	0.02%	0.003%
34	5.425	1345	1348	1349	rBV	228	148	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012326.D
 Acq On : 21 Aug 2019 20:45
 Operator : SY/MD
 Sample : K4464-03
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	5.453	1352	1357	1362	rVB3	350	369	0.05%	0.006%
36	5.531	1379	1381	1386	rBV	185	137	0.02%	0.002%
37	5.662	1408	1422	1447	rBV	249596	487970	60.76%	8.256%
38	5.945	1499	1510	1525	rVB3	9152	17583	2.19%	0.297%
39	6.003	1525	1528	1530	rBV	289	123	0.02%	0.002%
40	6.045	1537	1541	1543	rBV	222	191	0.02%	0.003%
41	6.116	1549	1563	1587	rBV	172857	341784	42.55%	5.783%
42	6.280	1612	1614	1620	rVB2	479	347	0.04%	0.006%
43	6.328	1625	1629	1632	rVB2	431	319	0.04%	0.005%
44	6.418	1655	1657	1658	rBV2	120	56	0.01%	0.001%
45	6.502	1682	1683	1684	rVB2	110	21	0.00%	0.000%
46	6.518	1684	1688	1691	rBV2	253	284	0.04%	0.005%
47	6.704	1742	1746	1750	rBV2	303	212	0.03%	0.004%
48	6.762	1760	1764	1768	rBV2	184	146	0.02%	0.002%
49	6.900	1804	1807	1808	rBV	156	109	0.01%	0.002%
50	6.978	1828	1831	1835	rBV	199	144	0.02%	0.002%
51	7.029	1835	1847	1865	rBV	108644	188578	23.48%	3.191%
52	7.177	1889	1893	1896	rBV	285	306	0.04%	0.005%
53	7.225	1907	1908	1913	rBV	232	108	0.01%	0.002%
54	7.264	1917	1920	1922	rBV	244	100	0.01%	0.002%
55	7.286	1925	1927	1929	rBV	156	105	0.01%	0.002%
56	7.357	1936	1949	1969	rBV	389129	671890	83.66%	11.368%
57	7.662	2033	2044	2060	rBV	74921	124942	15.56%	2.114%
58	7.965	2136	2138	2139	rBV	121	28	0.00%	0.000%
59	8.058	2165	2167	2169	rVB	207	107	0.01%	0.002%
60	8.129	2179	2189	2222	rBV2	159886	323978	40.34%	5.481%
61	8.408	2273	2276	2279	rBV2	190	136	0.02%	0.002%
62	8.428	2279	2282	2286	rBV	307	239	0.03%	0.004%
63	8.675	2356	2359	2362	rVV2	172	127	0.02%	0.002%
64	8.701	2363	2367	2371	rVB2	270	183	0.02%	0.003%
65	8.749	2379	2382	2383	rBV	192	106	0.01%	0.002%
66	8.849	2411	2413	2414	rBV	268	99	0.01%	0.002%
67	8.894	2415	2427	2456	rVV	355060	583154	72.61%	9.866%
68	9.270	2540	2544	2547	rVB	300	222	0.03%	0.004%
69	9.293	2547	2551	2555	rBV	252	240	0.03%	0.004%
70	9.341	2562	2566	2570	rVB2	273	295	0.04%	0.005%
71	9.485	2608	2611	2613	rBV2	158	97	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012326.D
 Acq On : 21 Aug 2019 20:45
 Operator : SY/MD
 Sample : K4464-03
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	9.553	2630	2632	2633	rBV	250	112	0.01%	0.002%
73	9.669	2664	2668	2671	rBV2	249	207	0.03%	0.004%
74	9.711	2677	2681	2687	rBV2	268	336	0.04%	0.006%
75	9.801	2706	2709	2710	rBV	145	87	0.01%	0.001%
76	9.887	2733	2736	2737	rBV	160	90	0.01%	0.002%
77	9.945	2750	2754	2757	rVB	279	223	0.03%	0.004%
78	9.977	2757	2764	2765	rBV2	350	347	0.04%	0.006%
79	10.032	2780	2781	2784	rVB	243	107	0.01%	0.002%
80	10.051	2784	2787	2790	rBV2	183	169	0.02%	0.003%
81	10.129	2807	2811	2812	rBV2	183	154	0.02%	0.003%
82	10.206	2832	2835	2838	rBV	245	200	0.02%	0.003%
83	10.260	2839	2852	2871	rVV2	236459	374345	46.61%	6.333%
84	10.379	2882	2889	2892	rBV	266	326	0.04%	0.006%
85	10.620	2962	2964	2967	rBV2	220	161	0.02%	0.003%
86	10.916	3053	3056	3058	rBV2	196	136	0.02%	0.002%
87	11.042	3092	3095	3097	rBV2	308	192	0.02%	0.003%
88	11.292	3161	3173	3197	rBV	323936	531962	66.23%	9.000%
89	11.669	3278	3290	3313	rBV	373832	611120	76.09%	10.339%
90	11.820	3335	3337	3338	rBV	202	59	0.01%	0.001%
91	11.833	3338	3341	3343	rBV	231	186	0.02%	0.003%
92	12.067	3412	3414	3416	rBV2	285	96	0.01%	0.002%
93	12.106	3423	3426	3427	rBV	189	131	0.02%	0.002%
94	12.691	3606	3608	3610	rBV	403	234	0.03%	0.004%
95	13.633	3899	3901	3902	rBV	299	124	0.02%	0.002%
96	14.035	4024	4026	4027	rBV	229	88	0.01%	0.001%


Sum of corrected areas: 5910595

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012326.D
Acq On : 21 Aug 2019 20:45
Operator : SY/MD
Sample : K4464-03
Misc : 5mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BEJW0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

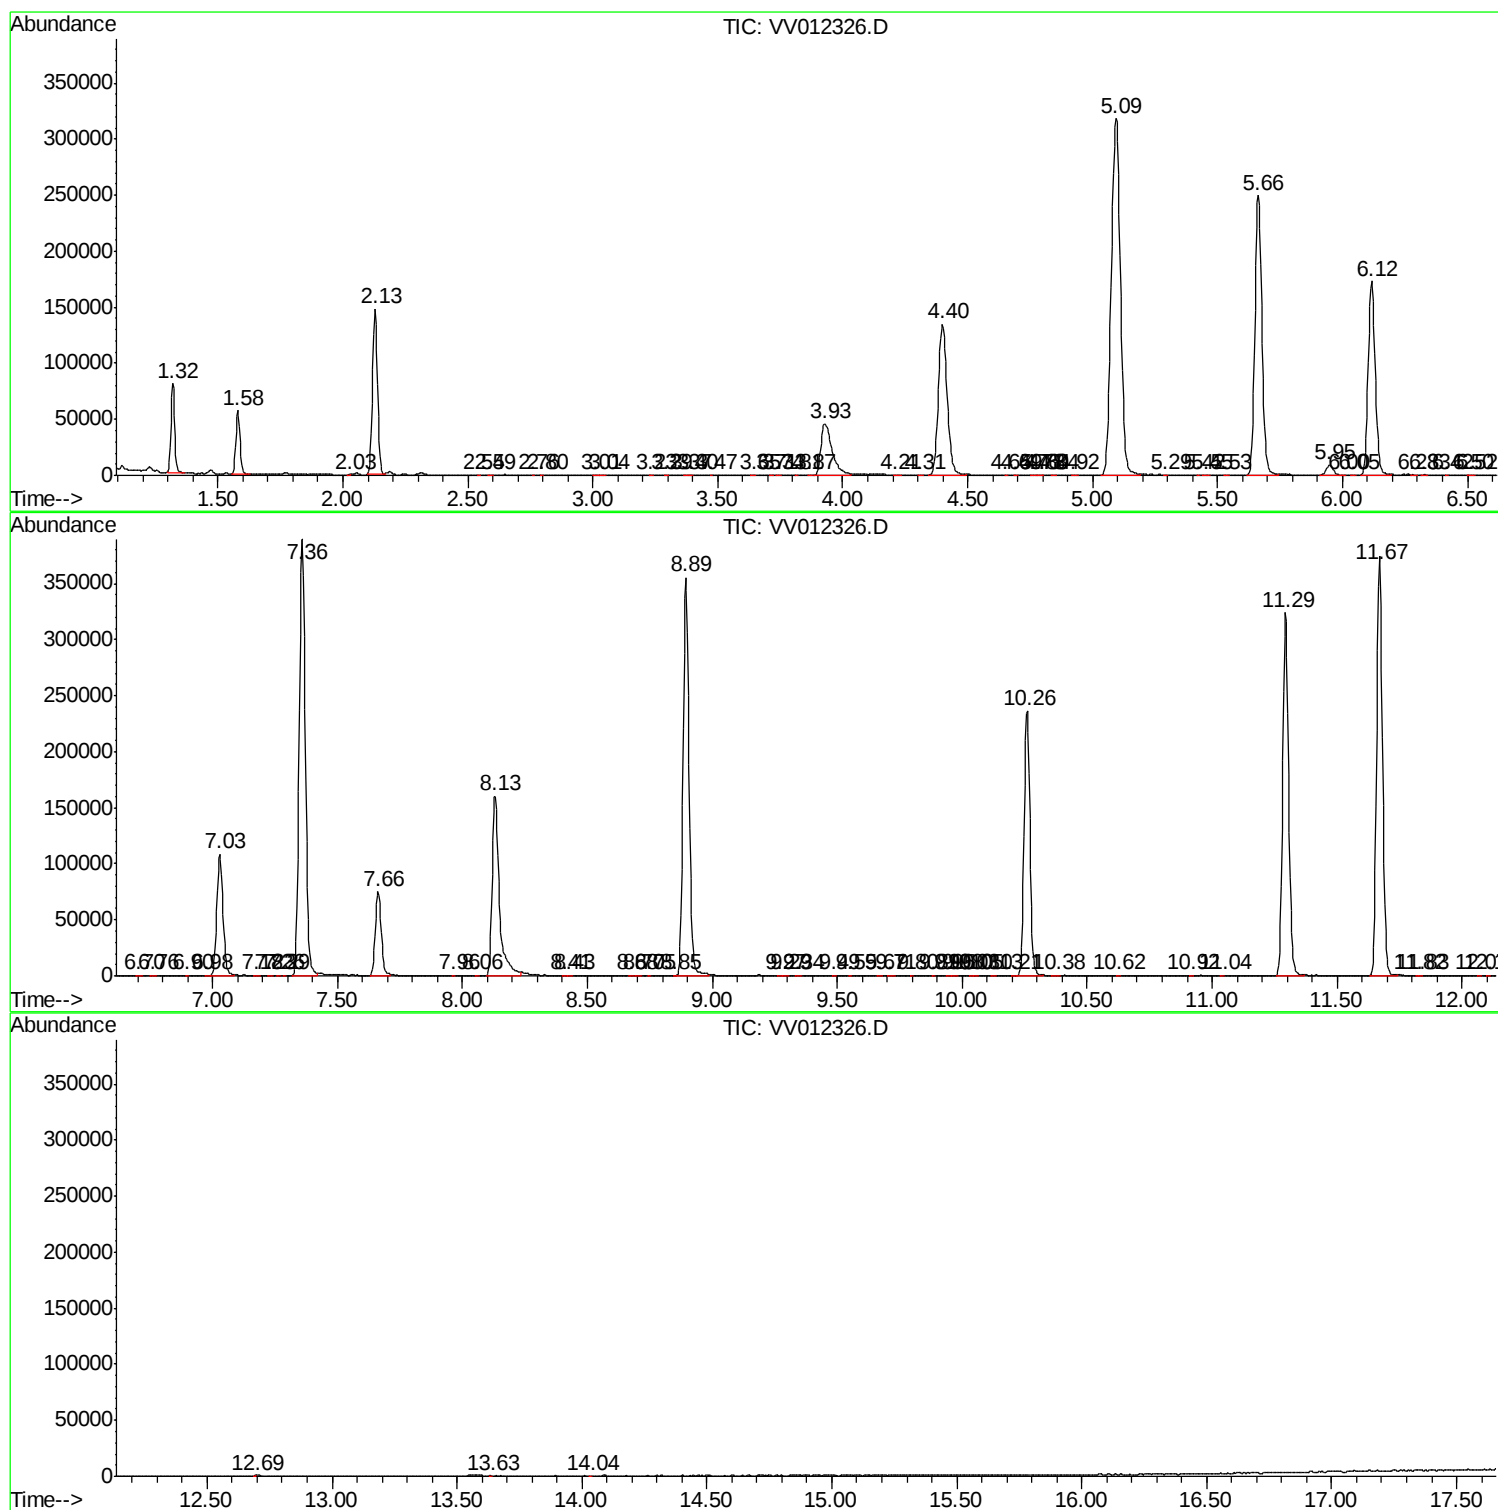

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082119\
Data File : VV012326.D
Acq On : 21 Aug 2019 20:45
Operator : SY/MD
Sample : K4464-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012326.D
Acq On : 21 Aug 2019 20:45
Operator : SY/MD
Sample : K4464-03
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEJW0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc