

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012327.D
 Acq On : 21 Aug 2019 21:09
 Operator : SY/MD
 Sample : K4464-04
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	88	rVB	84216	83215	10.25%	1.385%
2	1.579	144	152	167	rVB	57991	69226	8.53%	1.152%
3	1.962	269	271	275	rVB2	376	175	0.02%	0.003%
4	1.984	275	278	279	rBV2	404	249	0.03%	0.004%
5	2.052	291	299	306	rBV5	1485	2138	0.26%	0.036%
6	2.126	312	322	334	rBV	149892	213398	26.29%	3.551%
7	2.235	353	356	357	rBV3	558	339	0.04%	0.006%
8	2.399	405	407	408	rBV3	286	113	0.01%	0.002%
9	2.447	419	422	423	rBV	266	108	0.01%	0.002%
10	2.518	441	444	446	rBV	206	166	0.02%	0.003%
11	2.534	446	449	452	rVB	539	386	0.05%	0.006%
12	2.637	477	481	483	rBV2	184	115	0.01%	0.002%
13	2.897	559	562	565	rBV	174	87	0.01%	0.001%
14	3.103	625	626	630	rVB	164	100	0.01%	0.002%
15	3.129	632	634	638	rBV	242	143	0.02%	0.002%
16	3.164	642	645	646	rBV2	412	239	0.03%	0.004%
17	3.296	682	686	693	rVB2	367	451	0.06%	0.008%
18	3.524	755	757	760	rVB	191	95	0.01%	0.002%
19	3.547	760	764	767	rBV	194	186	0.02%	0.003%
20	3.614	782	785	789	rBV	247	201	0.02%	0.003%
21	3.798	833	842	845	rBV2	228	343	0.04%	0.006%
22	3.827	848	851	854	rBV2	173	128	0.02%	0.002%
23	3.852	856	859	861	rBV	243	149	0.02%	0.002%
24	3.865	861	863	866	rVB	213	78	0.01%	0.001%
25	3.926	870	882	918	rBV3	50288	150286	18.52%	2.501%
26	4.241	978	980	984	rBV	337	251	0.03%	0.004%
27	4.338	1007	1010	1011	rBV2	241	137	0.02%	0.002%
28	4.399	1013	1029	1059	rVB	138541	337129	41.54%	5.610%
29	4.569	1078	1082	1083	rBV	309	170	0.02%	0.003%
30	4.720	1126	1129	1136	rVB2	258	203	0.03%	0.003%
31	4.820	1158	1160	1164	rBV2	243	146	0.02%	0.002%
32	4.862	1171	1173	1176	rVB	178	78	0.01%	0.001%
33	4.894	1180	1183	1185	rBV	150	68	0.01%	0.001%
34	4.949	1198	1200	1206	rVB2	217	192	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012327.D
 Acq On : 21 Aug 2019 21:09
 Operator : SY/MD
 Sample : K4464-04
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	5.026	1222	1224	1226	rVB	133	68	0.01%	0.001%
36	5.093	1226	1245	1281	rBV2	321721	811590	100.00%	13.505%
37	5.296	1306	1308	1310	rVB	280	126	0.02%	0.002%
38	5.309	1310	1312	1314	rBV2	161	110	0.01%	0.002%
39	5.370	1327	1331	1333	rBV2	321	209	0.03%	0.003%
40	5.421	1344	1347	1349	rBV	219	164	0.02%	0.003%
41	5.444	1351	1354	1356	rBV2	193	121	0.01%	0.002%
42	5.454	1356	1357	1359	rBV2	242	89	0.01%	0.001%
43	5.502	1369	1372	1374	rBV	299	163	0.02%	0.003%
44	5.563	1389	1391	1396	rVB	230	146	0.02%	0.002%
45	5.614	1405	1407	1408	rBV	218	79	0.01%	0.001%
46	5.663	1408	1422	1444	rVV	251665	491366	60.54%	8.176%
47	5.897	1491	1495	1498	rBV3	254	228	0.03%	0.004%
48	5.949	1500	1511	1524	rVB5	8477	16758	2.06%	0.279%
49	6.116	1549	1563	1586	rBV	175299	349246	43.03%	5.811%
50	6.241	1600	1602	1603	rBV	379	186	0.02%	0.003%
51	6.286	1610	1616	1619	rVB2	179	199	0.02%	0.003%
52	6.428	1655	1660	1662	rBV	342	345	0.04%	0.006%
53	6.463	1667	1671	1672	rVV	128	105	0.01%	0.002%
54	6.540	1692	1695	1698	rVB2	212	138	0.02%	0.002%
55	6.634	1720	1724	1726	rBV	336	184	0.02%	0.003%
56	6.698	1742	1744	1753	rVB2	389	379	0.05%	0.006%
57	6.733	1753	1755	1757	rBV	160	87	0.01%	0.001%
58	6.759	1761	1763	1764	rBV	251	82	0.01%	0.001%
59	6.794	1771	1774	1779	rBV2	204	169	0.02%	0.003%
60	6.900	1804	1807	1811	rBV	192	140	0.02%	0.002%
61	7.029	1835	1847	1867	rBV	108213	188411	23.22%	3.135%
62	7.151	1882	1885	1890	rVB3	336	291	0.04%	0.005%
63	7.180	1892	1894	1896	rBV2	430	226	0.03%	0.004%
64	7.277	1922	1924	1931	rVB	207	196	0.02%	0.003%
65	7.357	1935	1949	1968	rBV	390538	682874	84.14%	11.363%
66	7.662	2033	2044	2066	rBV	77036	130034	16.02%	2.164%
67	7.859	2102	2105	2109	rBV2	187	175	0.02%	0.003%
68	7.987	2141	2145	2148	rVB	407	263	0.03%	0.004%
69	8.010	2149	2152	2154	rBV2	202	134	0.02%	0.002%
70	8.129	2178	2189	2222	rBV2	175101	344430	42.44%	5.731%
71	8.431	2278	2283	2286	rVB2	215	176	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012327.D
 Acq On : 21 Aug 2019 21:09
 Operator : SY/MD
 Sample : K4464-04
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	8.463	2290	2293	2296	rBV2	198	135	0.02%	0.002%
73	8.547	2317	2319	2325	rVB2	242	199	0.02%	0.003%
74	8.672	2355	2358	2359	rBV	193	111	0.01%	0.002%
75	8.740	2376	2379	2381	rBV2	168	102	0.01%	0.002%
76	8.894	2415	2427	2456	rBV	360007	589864	72.68%	9.815%
77	9.035	2469	2471	2473	rBV	247	125	0.02%	0.002%
78	9.061	2478	2479	2482	rVB2	242	113	0.01%	0.002%
79	9.264	2540	2542	2545	rBV2	226	142	0.02%	0.002%
80	9.367	2572	2574	2577	rBV2	161	107	0.01%	0.002%
81	9.466	2603	2605	2611	rVB	173	131	0.02%	0.002%
82	9.492	2611	2613	2615	rBV2	149	79	0.01%	0.001%
83	9.531	2622	2625	2626	rBV	202	109	0.01%	0.002%
84	9.588	2641	2643	2647	rVB3	608	468	0.06%	0.008%
85	9.624	2647	2654	2659	rBV2	444	731	0.09%	0.012%
86	9.723	2683	2685	2688	rVB	258	117	0.01%	0.002%
87	9.823	2712	2716	2720	rBV2	366	291	0.04%	0.005%
88	10.260	2840	2852	2874	rVB	238987	378471	46.63%	6.298%
89	10.498	2922	2926	2928	rBV2	157	129	0.02%	0.002%
90	10.656	2972	2975	2976	rBV	227	118	0.01%	0.002%
91	10.701	2986	2989	2991	rBV	157	110	0.01%	0.002%
92	11.122	3118	3120	3121	rBV	280	101	0.01%	0.002%
93	11.161	3130	3132	3135	rBV	248	132	0.02%	0.002%
94	11.293	3161	3173	3192	rBV	329597	535872	66.03%	8.917%
95	11.598	3265	3268	3270	rBV2	221	179	0.02%	0.003%
96	11.669	3278	3290	3309	rBV	384783	620861	76.50%	10.331%
97	11.884	3353	3357	3358	rBV	321	204	0.03%	0.003%
98	12.055	3407	3410	3413	rBV	266	260	0.03%	0.004%
99	14.074	4037	4038	4041	rBV	278	154	0.02%	0.003%
100	14.177	4069	4070	4072	rVB	253	90	0.01%	0.001%


Sum of corrected areas: 6009680

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012327.D
Acq On : 21 Aug 2019 21:09
Operator : SY/MD
Sample : K4464-04
Misc : 5mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

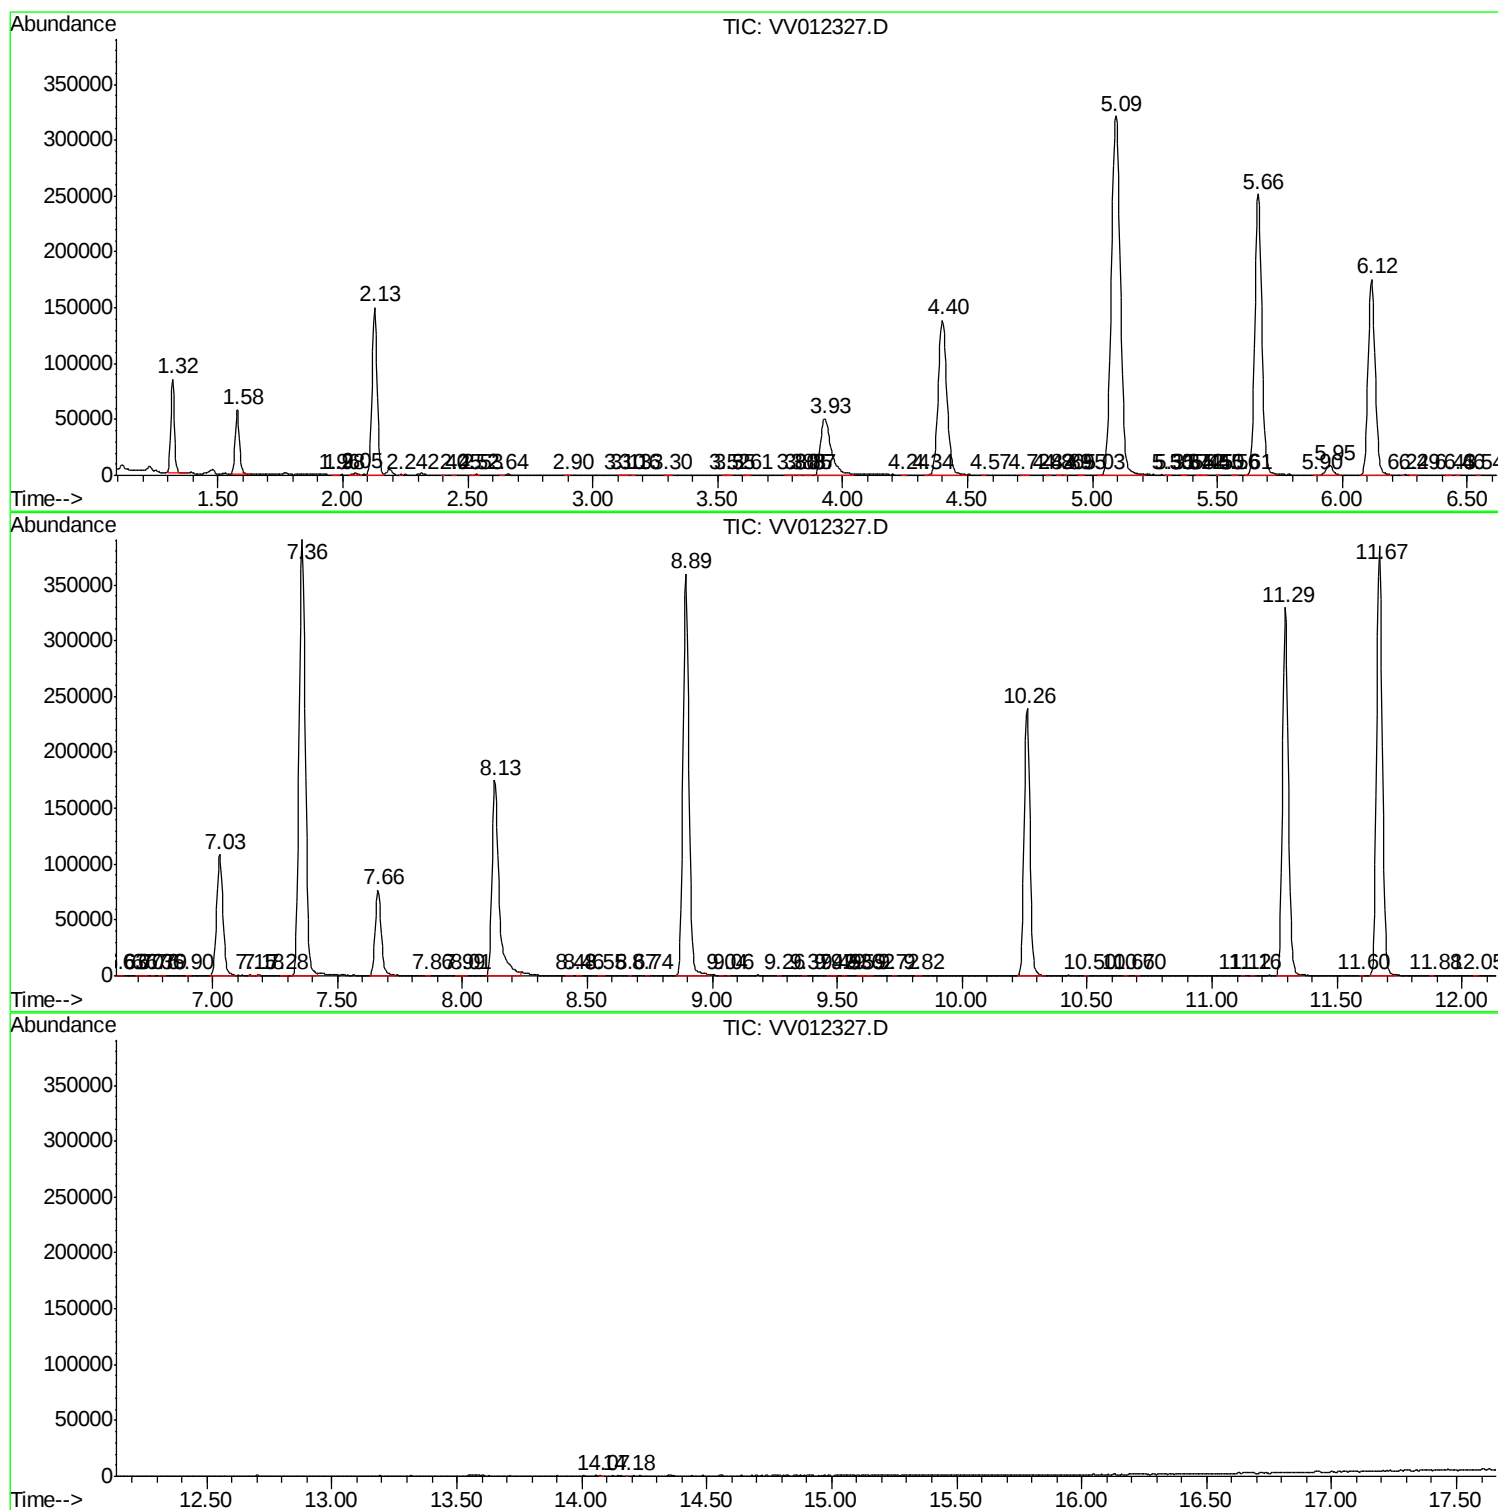

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082119\
Data File : VV012327.D
Acq On : 21 Aug 2019 21:09
Operator : SY/MD
Sample : K4464-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012327.D
Acq On : 21 Aug 2019 21:09
Operator : SY/MD
Sample : K4464-04
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEJW1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc