

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012328.D
 Acq On : 21 Aug 2019 21:34
 Operator : SY/MD
 Sample : K4464-05
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	79568	81725	10.23%	1.388%
2	1.579	145	152	168	rVB	56885	66945	8.38%	1.137%
3	1.769	206	211	220	rVB6	1994	2507	0.31%	0.043%
4	1.962	270	271	277	rVB3	286	135	0.02%	0.002%
5	2.052	292	299	306	rBV2	1633	2242	0.28%	0.038%
6	2.129	312	323	335	rBV	148092	210160	26.32%	3.570%
7	2.306	370	378	393	rVB2	3629	6725	0.84%	0.114%
8	2.531	445	448	456	rVB3	451	368	0.05%	0.006%
9	2.717	501	506	508	rBV2	171	165	0.02%	0.003%
10	2.765	516	521	527	rBV3	330	450	0.06%	0.008%
11	2.978	580	587	591	rVB2	251	322	0.04%	0.005%
12	3.003	591	595	597	rBV2	245	208	0.03%	0.004%
13	3.045	605	608	612	rVB2	279	220	0.03%	0.004%
14	3.106	621	627	631	rBV2	412	530	0.07%	0.009%
15	3.164	641	645	646	rBV	208	167	0.02%	0.003%
16	3.283	680	682	684	rBB	146	62	0.01%	0.001%
17	3.408	717	721	722	rBV	190	133	0.02%	0.002%
18	3.495	746	748	750	rVB	143	40	0.01%	0.001%
19	3.515	751	754	756	rBV	211	127	0.02%	0.002%
20	3.643	792	794	797	rBV	126	113	0.01%	0.002%
21	3.685	803	807	813	rVB2	283	257	0.03%	0.004%
22	3.743	822	825	827	rBV	209	111	0.01%	0.002%
23	3.759	828	830	831	rBV	117	44	0.01%	0.001%
24	3.798	839	842	845	rBV2	175	147	0.02%	0.002%
25	3.849	855	858	863	rBV2	181	139	0.02%	0.002%
26	3.929	870	883	919	rBV3	50100	147934	18.52%	2.513%
27	4.331	1006	1008	1009	rBV3	162	69	0.01%	0.001%
28	4.399	1012	1029	1053	rVV	136933	333025	41.70%	5.657%
29	4.540	1072	1073	1074	rBV	138	39	0.00%	0.001%
30	4.572	1081	1083	1084	rBV	163	49	0.01%	0.001%
31	4.582	1084	1086	1091	rVB3	351	277	0.03%	0.005%
32	4.701	1121	1123	1125	rBV	198	94	0.01%	0.002%
33	4.756	1136	1140	1141	rVB	230	105	0.01%	0.002%
34	4.769	1142	1144	1148	rVB2	254	153	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012328.D
 Acq On : 21 Aug 2019 21:34
 Operator : SY/MD
 Sample : K4464-05
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	4.849	1167	1169	1173	rVB	204	103	0.01%	0.002%
36	4.865	1173	1174	1175	rBV	127	30	0.00%	0.001%
37	4.897	1181	1184	1189	rBV2	200	229	0.03%	0.004%
38	4.939	1195	1197	1202	rVB	198	152	0.02%	0.003%
39	4.965	1202	1205	1207	rBV	256	194	0.02%	0.003%
40	4.994	1212	1214	1215	rBV2	112	63	0.01%	0.001%
41	5.093	1227	1245	1270	rBV2	316004	798578	100.00%	13.566%
42	5.299	1308	1309	1313	rVB2	324	93	0.01%	0.002%
43	5.498	1368	1371	1373	rBV	197	118	0.01%	0.002%
44	5.511	1373	1375	1378	rVV	230	121	0.02%	0.002%
45	5.524	1378	1379	1381	rVB	164	58	0.01%	0.001%
46	5.662	1408	1422	1451	rBV	242589	478864	59.96%	8.135%
47	5.949	1500	1511	1522	rBV3	9371	16885	2.11%	0.287%
48	6.116	1549	1563	1587	rBV	172542	342475	42.89%	5.818%
49	6.209	1591	1592	1594	rBV2	442	182	0.02%	0.003%
50	6.251	1603	1605	1607	rBV2	393	230	0.03%	0.004%
51	6.293	1615	1618	1620	rBV	306	190	0.02%	0.003%
52	6.367	1639	1641	1642	rVB	132	33	0.00%	0.001%
53	6.444	1662	1665	1666	rBV	189	81	0.01%	0.001%
54	6.630	1721	1723	1725	rBV	155	89	0.01%	0.002%
55	6.649	1727	1729	1732	rVV	343	189	0.02%	0.003%
56	6.685	1739	1740	1743	rBV	132	79	0.01%	0.001%
57	6.701	1743	1745	1746	rBV	138	36	0.00%	0.001%
58	6.746	1756	1759	1762	rBV2	173	127	0.02%	0.002%
59	6.830	1782	1785	1787	rBV	165	115	0.01%	0.002%
60	6.913	1809	1811	1814	rBV	152	65	0.01%	0.001%
61	6.936	1814	1818	1821	rBV2	161	162	0.02%	0.003%
62	6.977	1829	1831	1833	rVB	148	41	0.01%	0.001%
63	7.029	1834	1847	1860	rBV	108230	186911	23.41%	3.175%
64	7.199	1898	1900	1902	rVB	337	95	0.01%	0.002%
65	7.228	1905	1909	1912	rVB3	302	223	0.03%	0.004%
66	7.360	1936	1950	1968	rBV	386105	670706	83.99%	11.393%
67	7.662	2033	2044	2061	rBV	73877	126412	15.83%	2.147%
68	7.875	2108	2110	2112	rVB	143	56	0.01%	0.001%
69	7.894	2114	2116	2118	rBV	165	86	0.01%	0.001%
70	7.910	2118	2121	2124	rVB	170	96	0.01%	0.002%
71	7.932	2125	2128	2130	rBV2	378	227	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012328.D
 Acq On : 21 Aug 2019 21:34
 Operator : SY/MD
 Sample : K4464-05
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	8.087	2171	2176	2178	rBV2	332	335	0.04%	0.006%
73	8.129	2178	2189	2216	rBV4	164360	330274	41.36%	5.610%
74	8.402	2271	2274	2278	rBV	225	178	0.02%	0.003%
75	8.511	2306	2308	2309	rBV	273	96	0.01%	0.002%
76	8.624	2337	2343	2344	rBV	200	188	0.02%	0.003%
77	8.707	2365	2369	2371	rBV	167	130	0.02%	0.002%
78	8.730	2374	2376	2377	rBV	153	82	0.01%	0.001%
79	8.791	2392	2395	2397	rVB	220	120	0.02%	0.002%
80	8.826	2403	2406	2407	rBV2	137	97	0.01%	0.002%
81	8.894	2414	2427	2458	rBV	350998	569251	71.28%	9.670%
82	9.315	2555	2558	2561	rBV	175	116	0.01%	0.002%
83	9.379	2573	2578	2586	rBV2	269	534	0.07%	0.009%
84	9.556	2629	2633	2636	rBV	200	193	0.02%	0.003%
85	9.749	2691	2693	2696	rVB2	138	76	0.01%	0.001%
86	9.788	2696	2705	2708	rBV2	240	364	0.05%	0.006%
87	9.897	2736	2739	2741	rBV	218	186	0.02%	0.003%
88	9.977	2760	2764	2767	rBV2	383	386	0.05%	0.007%
89	10.186	2827	2829	2830	rBV	138	76	0.01%	0.001%
90	10.260	2839	2852	2874	rVB	233771	374564	46.90%	6.363%
91	10.392	2891	2893	2896	rBV	203	137	0.02%	0.002%
92	10.418	2898	2901	2903	rBV	228	159	0.02%	0.003%
93	10.524	2931	2934	2936	rBV2	210	177	0.02%	0.003%
94	10.749	3001	3004	3006	rBV	200	120	0.02%	0.002%
95	11.292	3161	3173	3194	rBV	319311	516158	64.63%	8.768%
96	11.672	3278	3291	3309	rBV	375733	611914	76.63%	10.395%
97	11.919	3364	3368	3370	rBV2	365	343	0.04%	0.006%
98	12.173	3443	3447	3449	rBV	291	233	0.03%	0.004%
99	13.257	3782	3784	3785	rBV	157	67	0.01%	0.001%
100	13.971	4004	4006	4007	rBV	313	87	0.01%	0.001%


Sum of corrected areas: 5886822

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012328.D
Acq On : 21 Aug 2019 21:34
Operator : SY/MD
Sample : K4464-05
Misc : 5mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

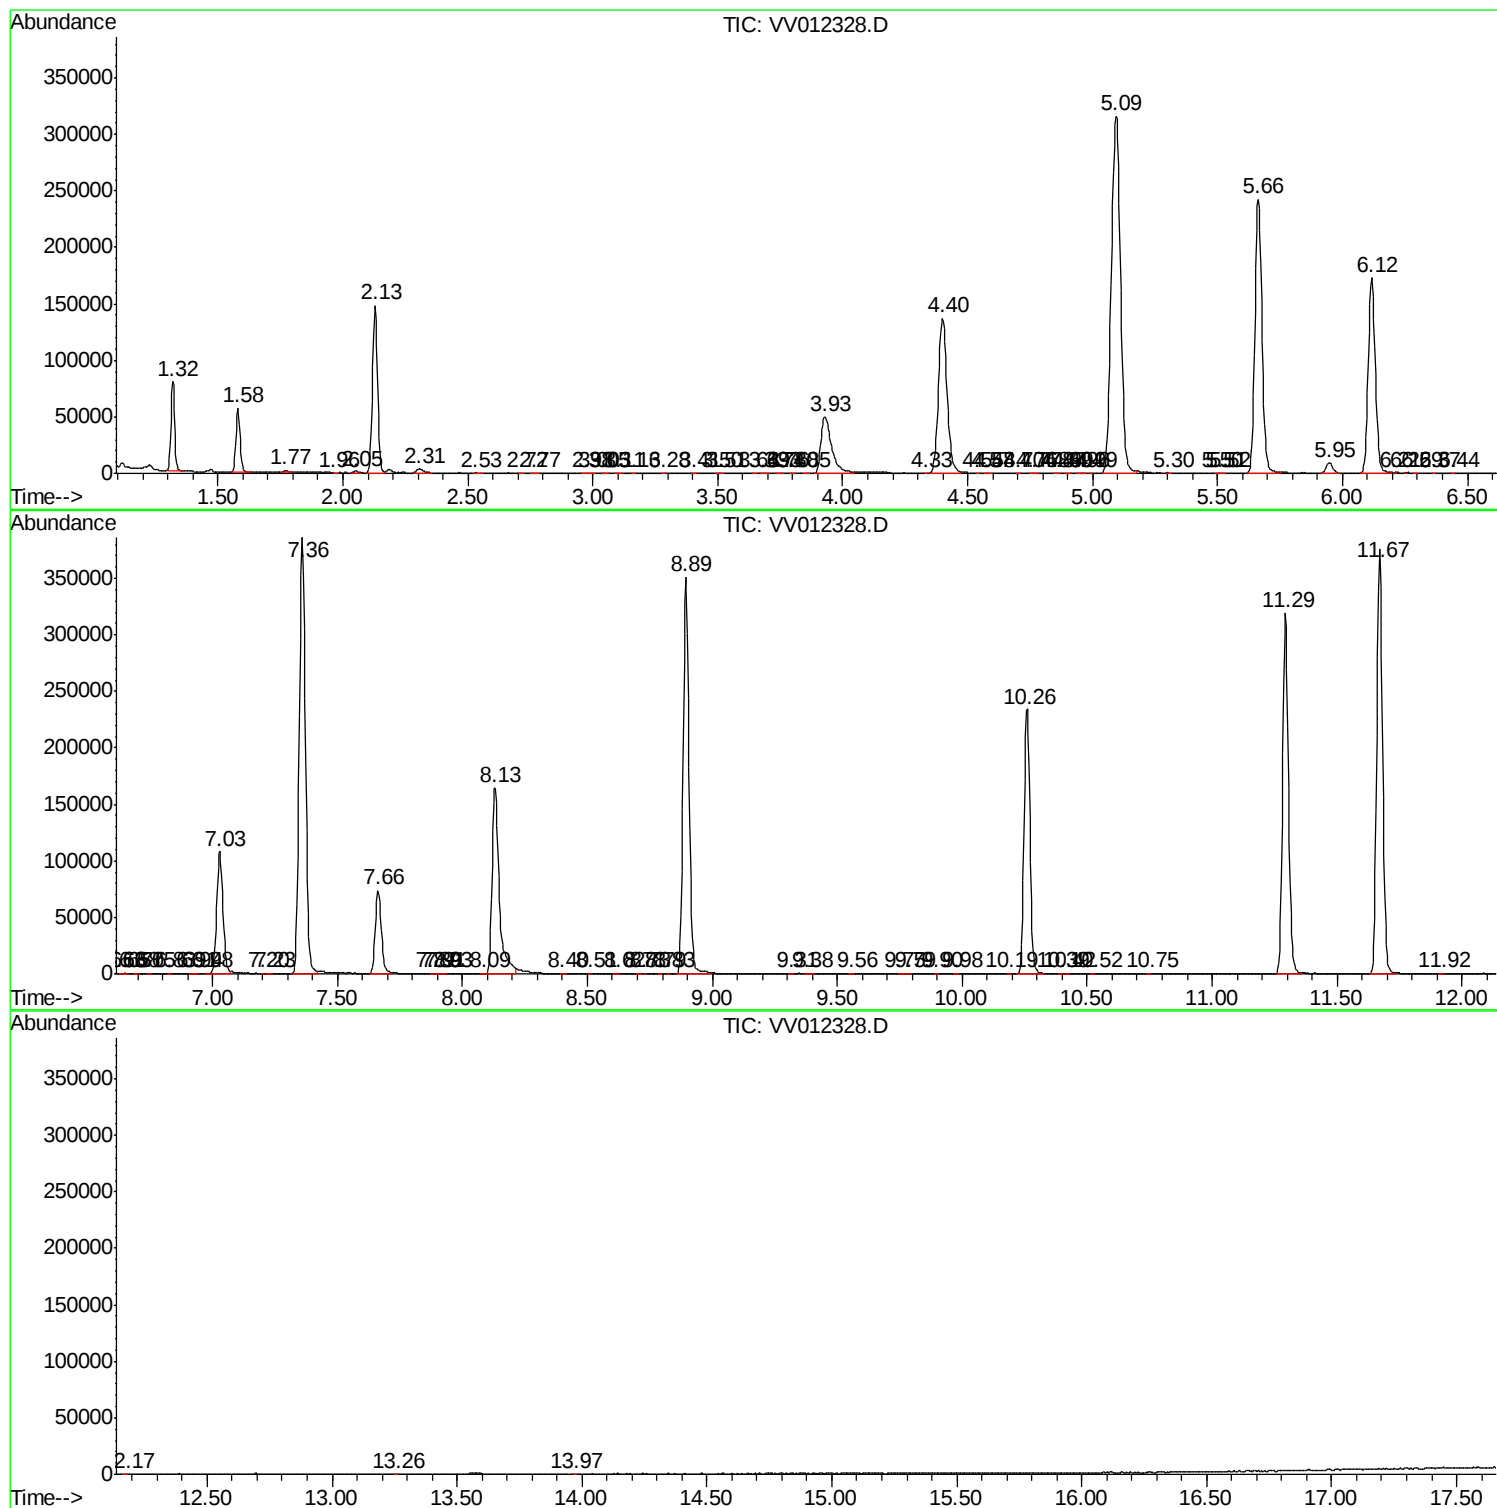

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012328.D
Acq On : 21 Aug 2019 21:34
Operator : SY/MD
Sample : K4464-05
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEJW2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012328.D
Acq On : 21 Aug 2019 21:34
Operator : SY/MD
Sample : K4464-05
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEJW2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc