

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012329.D
 Acq On : 21 Aug 2019 21:58
 Operator : SY/MD
 Sample : K4464-08
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	88	rVB	79917	83399	10.56%	1.412%
2	1.579	145	152	164	rVB	56720	66601	8.43%	1.127%
3	1.769	207	211	217	rVB3	2046	2272	0.29%	0.038%
4	1.987	276	279	281	rBV2	373	208	0.03%	0.004%
5	2.129	312	323	335	rBV	147824	208882	26.45%	3.536%
6	2.309	370	379	392	rVB5	2205	3981	0.50%	0.067%
7	2.531	446	448	450	rBV	380	226	0.03%	0.004%
8	2.569	457	460	463	rBV2	236	180	0.02%	0.003%
9	2.634	479	480	483	rVB	222	65	0.01%	0.001%
10	2.663	487	489	491	rBV	248	127	0.02%	0.002%
11	2.769	518	522	525	rBV2	364	429	0.05%	0.007%
12	2.852	546	548	549	rBV2	238	119	0.02%	0.002%
13	2.962	579	582	584	rBV	194	156	0.02%	0.003%
14	3.048	606	609	611	rBV	147	92	0.01%	0.002%
15	3.155	639	642	643	rBV	149	83	0.01%	0.001%
16	3.180	647	650	654	rBV	181	146	0.02%	0.002%
17	3.200	654	656	657	rBV	200	59	0.01%	0.001%
18	3.238	665	668	672	rVB2	188	146	0.02%	0.002%
19	3.261	672	675	679	rBV	204	190	0.02%	0.003%
20	3.309	685	690	693	rBV2	270	285	0.04%	0.005%
21	3.383	709	713	715	rBV2	266	222	0.03%	0.004%
22	3.534	757	760	762	rBV2	258	193	0.02%	0.003%
23	3.550	762	765	766	rVV	223	119	0.02%	0.002%
24	3.589	774	777	780	rVB	184	129	0.02%	0.002%
25	3.630	787	790	792	rBV	159	106	0.01%	0.002%
26	3.794	840	841	844	rVB	123	58	0.01%	0.001%
27	3.839	853	855	859	rVB	187	74	0.01%	0.001%
28	3.859	859	861	863	rBV	357	161	0.02%	0.003%
29	3.926	870	882	915	rBV2	49004	143344	18.15%	2.426%
30	4.277	987	991	994	rVB2	396	312	0.04%	0.005%
31	4.335	1007	1009	1011	rBV	192	93	0.01%	0.002%
32	4.399	1011	1029	1059	rVV	133907	330740	41.88%	5.598%
33	4.543	1073	1074	1075	rBV	240	83	0.01%	0.001%
34	4.701	1121	1123	1126	rBV	207	112	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012329.D
 Acq On : 21 Aug 2019 21:58
 Operator : SY/MD
 Sample : K4464-08
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	4.814	1154	1158	1163	rBV2	321	377	0.05%	0.006%
36	4.897	1181	1184	1187	rBV	189	116	0.01%	0.002%
37	4.949	1198	1200	1202	rBV	113	68	0.01%	0.001%
38	5.003	1215	1217	1219	rBV	133	82	0.01%	0.001%
39	5.093	1226	1245	1266	rBV2	314490	789664	100.00%	13.366%
40	5.370	1329	1331	1333	rBV2	218	107	0.01%	0.002%
41	5.434	1345	1351	1355	rBV3	378	450	0.06%	0.008%
42	5.479	1360	1365	1369	rBV2	311	308	0.04%	0.005%
43	5.511	1371	1375	1378	rBV	240	229	0.03%	0.004%
44	5.585	1396	1398	1405	rVB2	198	179	0.02%	0.003%
45	5.662	1408	1422	1443	rBV	254502	493075	62.44%	8.346%
46	5.875	1485	1488	1489	rBV	291	186	0.02%	0.003%
47	5.949	1501	1511	1528	rVB3	8986	17964	2.27%	0.304%
48	6.023	1529	1534	1536	rBV	272	220	0.03%	0.004%
49	6.116	1550	1563	1587	rBV2	171489	341340	43.23%	5.778%
50	6.212	1591	1593	1596	rBV2	330	156	0.02%	0.003%
51	6.334	1629	1631	1635	rVB	203	140	0.02%	0.002%
52	6.473	1671	1674	1677	rBV	189	94	0.01%	0.002%
53	6.608	1714	1716	1719	rBV	255	210	0.03%	0.004%
54	6.637	1722	1725	1727	rBV2	162	119	0.02%	0.002%
55	6.704	1742	1746	1750	rBV	363	359	0.05%	0.006%
56	6.727	1750	1753	1754	rBV2	201	116	0.01%	0.002%
57	6.814	1777	1780	1783	rBV	173	111	0.01%	0.002%
58	7.029	1836	1847	1861	rBV	105782	182891	23.16%	3.096%
59	7.219	1904	1906	1907	rBV	129	54	0.01%	0.001%
60	7.273	1919	1923	1927	rVB2	221	191	0.02%	0.003%
61	7.357	1935	1949	1969	rBV	380499	660446	83.64%	11.179%
62	7.608	2024	2027	2028	rBV	267	114	0.01%	0.002%
63	7.662	2033	2044	2067	rBV	74446	126730	16.05%	2.145%
64	7.833	2094	2097	2100	rBV	269	208	0.03%	0.004%
65	7.961	2135	2137	2141	rVB2	152	84	0.01%	0.001%
66	7.987	2141	2145	2147	rBV2	345	284	0.04%	0.005%
67	8.058	2165	2167	2170	rVB	172	79	0.01%	0.001%
68	8.077	2170	2173	2175	rBV	234	159	0.02%	0.003%
69	8.129	2178	2189	2222	rBV2	162132	328761	41.63%	5.565%
70	8.357	2258	2260	2261	rBV	157	85	0.01%	0.001%
71	8.421	2277	2280	2283	rBV	246	219	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012329.D
 Acq On : 21 Aug 2019 21:58
 Operator : SY/MD
 Sample : K4464-08
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEJW3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	8.434	2283	2284	2285	rVV	236	56	0.01%	0.001%
73	8.672	2355	2358	2360	rBV2	185	107	0.01%	0.002%
74	8.688	2360	2363	2366	rVB2	312	216	0.03%	0.004%
75	8.707	2366	2369	2373	rBV2	220	218	0.03%	0.004%
76	8.801	2396	2398	2400	rBV2	198	137	0.02%	0.002%
77	8.842	2407	2411	2414	rBV2	204	149	0.02%	0.003%
78	8.894	2414	2427	2471	rVB	363466	597588	75.68%	10.115%
79	9.058	2471	2478	2481	rBV3	357	433	0.05%	0.007%
80	9.090	2484	2488	2491	rBV	247	230	0.03%	0.004%
81	9.257	2538	2540	2542	rBV	195	127	0.02%	0.002%
82	9.411	2586	2588	2593	rBV	189	159	0.02%	0.003%
83	9.534	2623	2626	2628	rBV2	199	111	0.01%	0.002%
84	9.585	2636	2642	2643	rBV2	350	296	0.04%	0.005%
85	9.669	2664	2668	2670	rBV	256	213	0.03%	0.004%
86	9.759	2691	2696	2700	rBV2	291	367	0.05%	0.006%
87	9.833	2717	2719	2721	rVB	189	72	0.01%	0.001%
88	9.849	2721	2724	2728	rBV	290	249	0.03%	0.004%
89	9.952	2753	2756	2759	rBV	256	205	0.03%	0.003%
90	10.000	2768	2771	2773	rBV	382	248	0.03%	0.004%
91	10.154	2816	2819	2822	rBV	250	173	0.02%	0.003%
92	10.260	2840	2852	2877	rVB	238866	371549	47.05%	6.289%
93	10.350	2877	2880	2881	rBV2	179	125	0.02%	0.002%
94	10.389	2890	2892	2894	rBV	267	115	0.01%	0.002%
95	10.453	2909	2912	2916	rBV2	182	201	0.03%	0.003%
96	10.704	2987	2990	2994	rBV2	255	256	0.03%	0.004%
97	11.292	3161	3173	3193	rBV	332116	535285	67.79%	9.061%
98	11.669	3278	3290	3312	rBV	373012	609192	77.15%	10.312%
99	13.389	3823	3825	3829	rBV2	255	148	0.02%	0.003%
100	13.681	3913	3916	3919	rBV2	251	207	0.03%	0.004%


Sum of corrected areas: 5907799

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012329.D
Acq On : 21 Aug 2019 21:58
Operator : SY/MD
Sample : K4464-08
Misc : 5mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

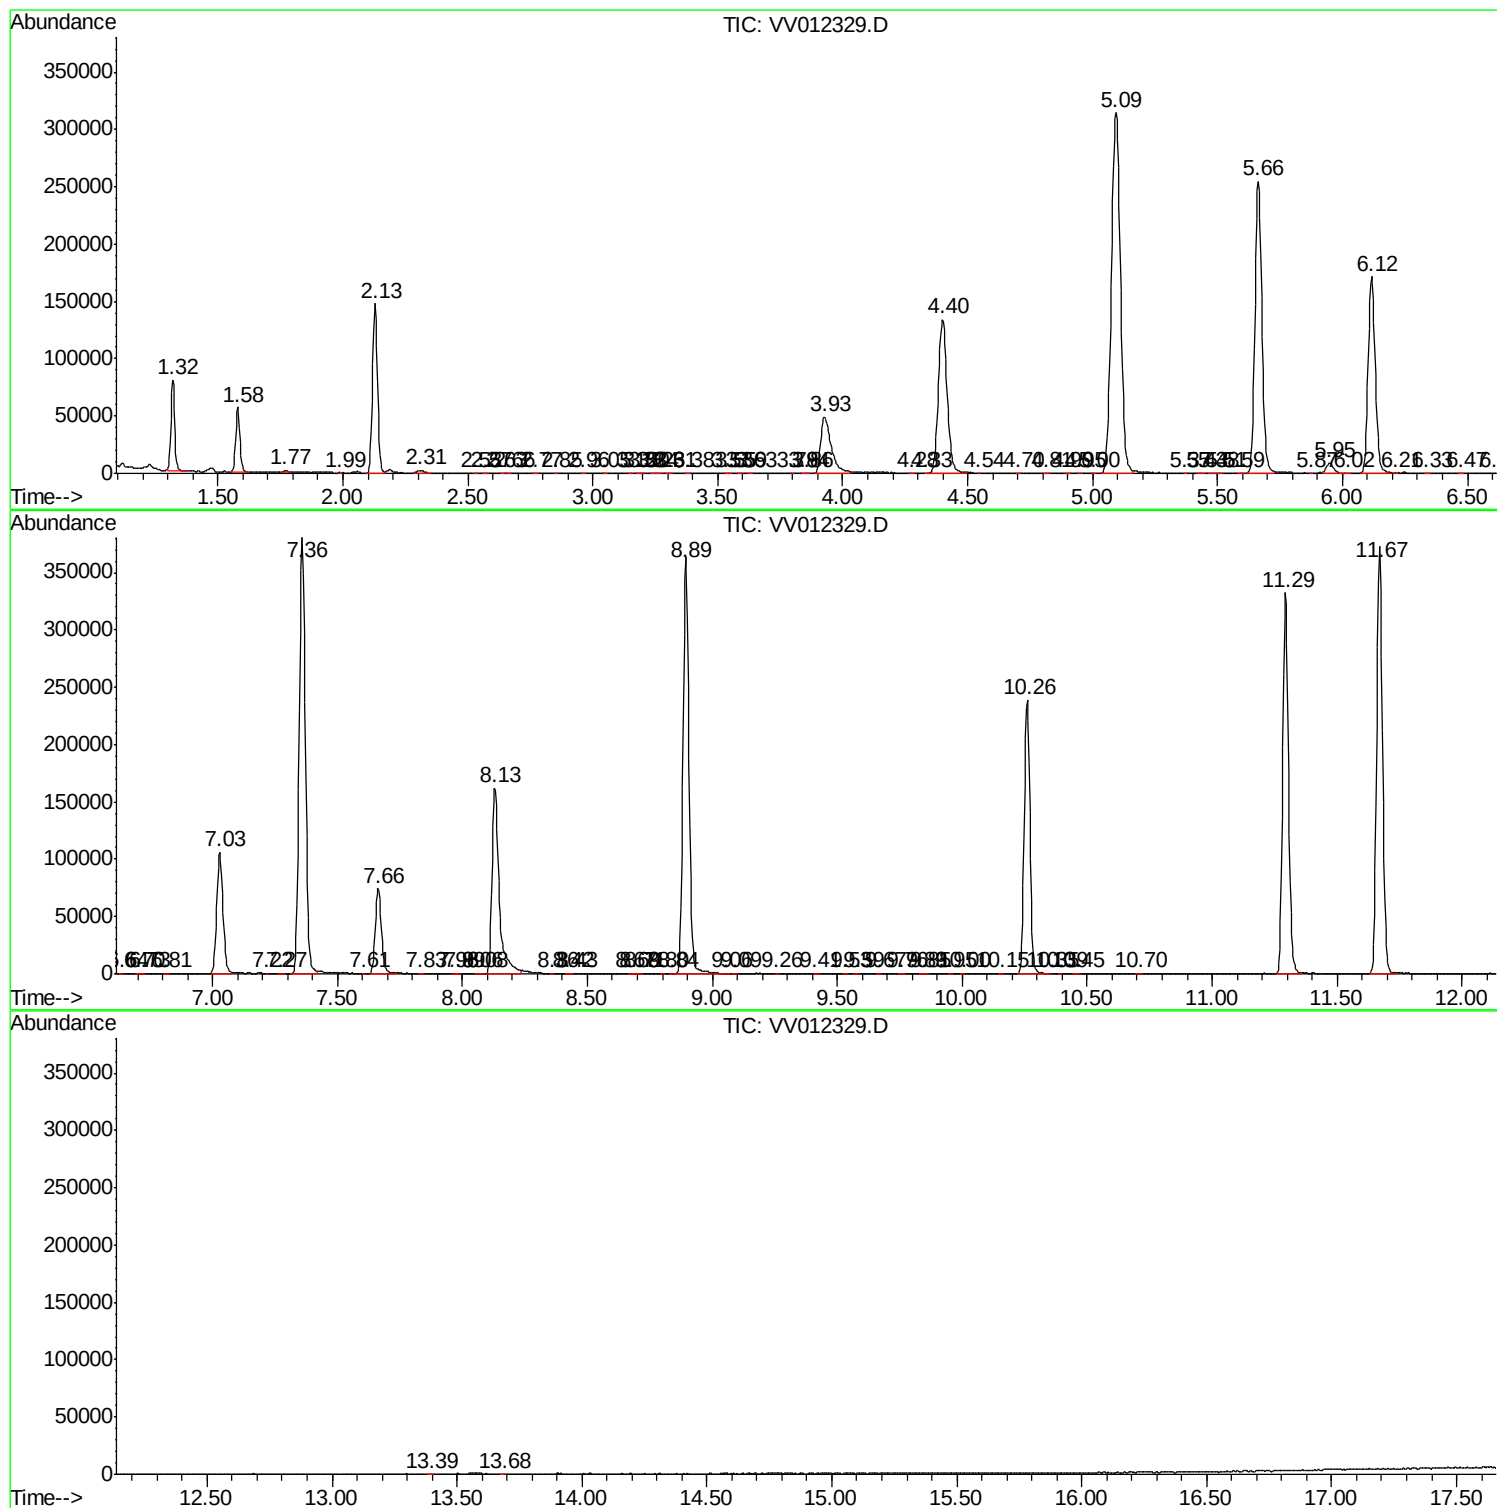

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082119\
Data File : VV012329.D
Acq On : 21 Aug 2019 21:58
Operator : SY/MD
Sample : K4464-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEJW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012329.D
Acq On : 21 Aug 2019 21:58
Operator : SY/MD
Sample : K4464-08
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEJW3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
