

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012332.D
 Acq On : 21 Aug 2019 23:12
 Operator : SY/MD
 Sample : K4454-11
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2C03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	87	rVB	81537	85119	10.69%	1.407%
2	1.579	145	152	163	rVB	55980	64556	8.11%	1.067%
3	2.052	290	299	304	rBV5	1602	1922	0.24%	0.032%
4	2.126	311	322	334	rBV	146123	207846	26.11%	3.436%
5	2.463	423	427	428	rBV	327	251	0.03%	0.004%
6	2.618	472	475	477	rBV2	216	132	0.02%	0.002%
7	2.656	479	487	501	rVV2	5316	9073	1.14%	0.150%
8	2.801	522	532	545	rVB2	18310	36289	4.56%	0.600%
9	2.978	584	587	589	rBV2	154	103	0.01%	0.002%
10	3.042	605	607	610	rVB	157	68	0.01%	0.001%
11	3.058	610	612	614	rBV	191	93	0.01%	0.002%
12	3.132	632	635	641	rBV2	265	300	0.04%	0.005%
13	3.183	648	651	654	rBV2	161	144	0.02%	0.002%
14	3.238	665	668	673	rVB2	229	197	0.02%	0.003%
15	3.264	673	676	677	rBV	159	94	0.01%	0.002%
16	3.344	698	701	702	rBV	119	55	0.01%	0.001%
17	3.457	733	736	737	rBV	145	59	0.01%	0.001%
18	3.482	742	744	746	rBV	143	75	0.01%	0.001%
19	3.524	754	757	759	rBV	216	164	0.02%	0.003%
20	3.553	764	766	767	rVB	209	68	0.01%	0.001%
21	3.569	768	771	774	rBV	168	144	0.02%	0.002%
22	3.601	779	781	785	rVB	180	94	0.01%	0.002%
23	3.624	785	788	791	rBV2	238	230	0.03%	0.004%
24	3.659	797	799	802	rBV	154	122	0.02%	0.002%
25	3.753	826	828	830	rBV	170	91	0.01%	0.002%
26	3.772	830	834	837	rVB	189	140	0.02%	0.002%
27	3.814	843	847	851	rVB2	264	220	0.03%	0.004%
28	3.836	851	854	859	rBV2	149	124	0.02%	0.002%
29	3.868	861	864	869	rBV	237	168	0.02%	0.003%
30	3.955	869	891	918	rBV4	76081	281432	35.36%	4.653%
31	4.116	938	941	943	rBV	396	267	0.03%	0.004%
32	4.309	999	1001	1002	rBV	134	52	0.01%	0.001%
33	4.399	1012	1029	1060	rBV	131877	333744	41.93%	5.518%
34	4.589	1086	1088	1091	rVB2	228	127	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012332.D
 Acq On : 21 Aug 2019 23:12
 Operator : SY/MD
 Sample : K4454-11
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2C03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	4.630	1094	1101	1102	rBV	230	260	0.03%	0.004%
36	4.643	1102	1105	1107	rVB2	229	126	0.02%	0.002%
37	4.714	1123	1127	1130	rBV2	217	192	0.02%	0.003%
38	4.868	1172	1175	1178	rBV	287	199	0.03%	0.003%
39	4.942	1195	1198	1200	rBV2	222	175	0.02%	0.003%
40	5.093	1224	1245	1270	rBV2	318054	795986	100.00%	13.160%
41	5.383	1332	1335	1337	rBV	245	142	0.02%	0.002%
42	5.460	1356	1359	1360	rVV	341	119	0.01%	0.002%
43	5.470	1360	1362	1366	rVB	228	169	0.02%	0.003%
44	5.521	1375	1378	1381	rVB	321	190	0.02%	0.003%
45	5.534	1381	1382	1383	rBV	222	49	0.01%	0.001%
46	5.592	1397	1400	1403	rBV	188	117	0.01%	0.002%
47	5.662	1408	1422	1449	rBV	239406	477599	60.00%	7.896%
48	5.945	1499	1510	1525	rVB5	9232	16505	2.07%	0.273%
49	6.058	1543	1545	1547	rBV	199	112	0.01%	0.002%
50	6.116	1547	1563	1587	rVV	175698	344552	43.29%	5.696%
51	6.289	1614	1617	1618	rBV	146	66	0.01%	0.001%
52	6.302	1618	1621	1623	rVV	258	151	0.02%	0.002%
53	6.511	1684	1686	1688	rBV	144	102	0.01%	0.002%
54	6.605	1713	1715	1718	rBV	234	123	0.02%	0.002%
55	6.624	1718	1721	1724	rBV	164	126	0.02%	0.002%
56	6.794	1770	1774	1776	rBV	164	128	0.02%	0.002%
57	6.846	1784	1790	1793	rVV2	258	320	0.04%	0.005%
58	6.865	1793	1796	1798	rBV	128	80	0.01%	0.001%
59	6.881	1798	1801	1803	rBV	205	152	0.02%	0.003%
60	6.939	1817	1819	1820	rVB2	258	68	0.01%	0.001%
61	6.984	1831	1833	1835	rBV	183	90	0.01%	0.001%
62	7.029	1835	1847	1868	rVV	103952	184165	23.14%	3.045%
63	7.151	1882	1885	1890	rVB2	464	369	0.05%	0.006%
64	7.248	1912	1915	1916	rBV2	230	135	0.02%	0.002%
65	7.286	1925	1927	1931	rVB2	218	142	0.02%	0.002%
66	7.312	1932	1935	1937	rBV2	215	128	0.02%	0.002%
67	7.360	1937	1950	1968	rBV	382627	663806	83.39%	10.975%
68	7.608	2024	2027	2029	rBV	168	109	0.01%	0.002%
69	7.662	2033	2044	2064	rVV	74717	122722	15.42%	2.029%
70	7.974	2139	2141	2143	rBV	226	156	0.02%	0.003%
71	8.061	2165	2168	2171	rBV2	222	133	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012332.D
Acq On : 21 Aug 2019 23:12
Operator : SY/MD
Sample : K4454-11
Misc : 5mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2C03

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Title : VOC Analysis

72	8.129	2178	2189	2215	rBV2	163215	322097	40.47%	5.325%
73	8.376	2264	2266	2270	rBV2	214	186	0.02%	0.003%
74	8.457	2289	2291	2293	rBV	131	53	0.01%	0.001%
75	8.537	2313	2316	2321	rBV	397	340	0.04%	0.006%
76	8.894	2415	2427	2465	rBV	350335	570270	71.64%	9.428%
77	9.180	2509	2516	2523	rBV2	1035	1617	0.20%	0.027%
78	9.231	2529	2532	2533	rBV	196	109	0.01%	0.002%
79	9.273	2542	2545	2548	rBV	231	162	0.02%	0.003%
80	9.321	2559	2560	2565	rBV2	261	139	0.02%	0.002%
81	9.620	2650	2653	2656	rBV3	283	209	0.03%	0.003%
82	9.743	2688	2691	2693	rVB2	175	94	0.01%	0.002%
83	9.762	2694	2697	2703	rBV2	233	305	0.04%	0.005%
84	9.939	2750	2752	2755	rBV	286	156	0.02%	0.003%
85	10.032	2775	2781	2782	rBV2	382	400	0.05%	0.007%
86	10.260	2840	2852	2871	rBV	236129	373272	46.89%	6.171%
87	10.373	2879	2887	2893	rBV2	323	532	0.07%	0.009%
88	10.418	2897	2901	2905	rBV	216	206	0.03%	0.003%
89	10.440	2905	2908	2913	rBV2	269	215	0.03%	0.004%
90	10.582	2949	2952	2959	rVB2	614	589	0.07%	0.010%
91	10.617	2959	2963	2966	rBV2	240	233	0.03%	0.004%
92	10.810	3022	3023	3025	rBV2	223	80	0.01%	0.001%
93	10.839	3028	3032	3034	rBV	403	262	0.03%	0.004%
94	11.080	3105	3107	3109	rBV	151	79	0.01%	0.001%
95	11.100	3109	3113	3116	rBV	342	300	0.04%	0.005%
96	11.292	3161	3173	3196	rBV	325008	524483	65.89%	8.671%
97	11.569	3257	3259	3260	rBV	387	126	0.02%	0.002%
98	11.669	3278	3290	3318	rBV	381078	618466	77.70%	10.225%
99	14.196	4075	4076	4077	rBV	268	64	0.01%	0.001%
100	14.656	4216	4219	4221	rBV	296	168	0.02%	0.003%


Sum of corrected areas: 6048538

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012332.D
Acq On : 21 Aug 2019 23:12
Operator : SY/MD
Sample : K4454-11
Misc : 5mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2C03

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

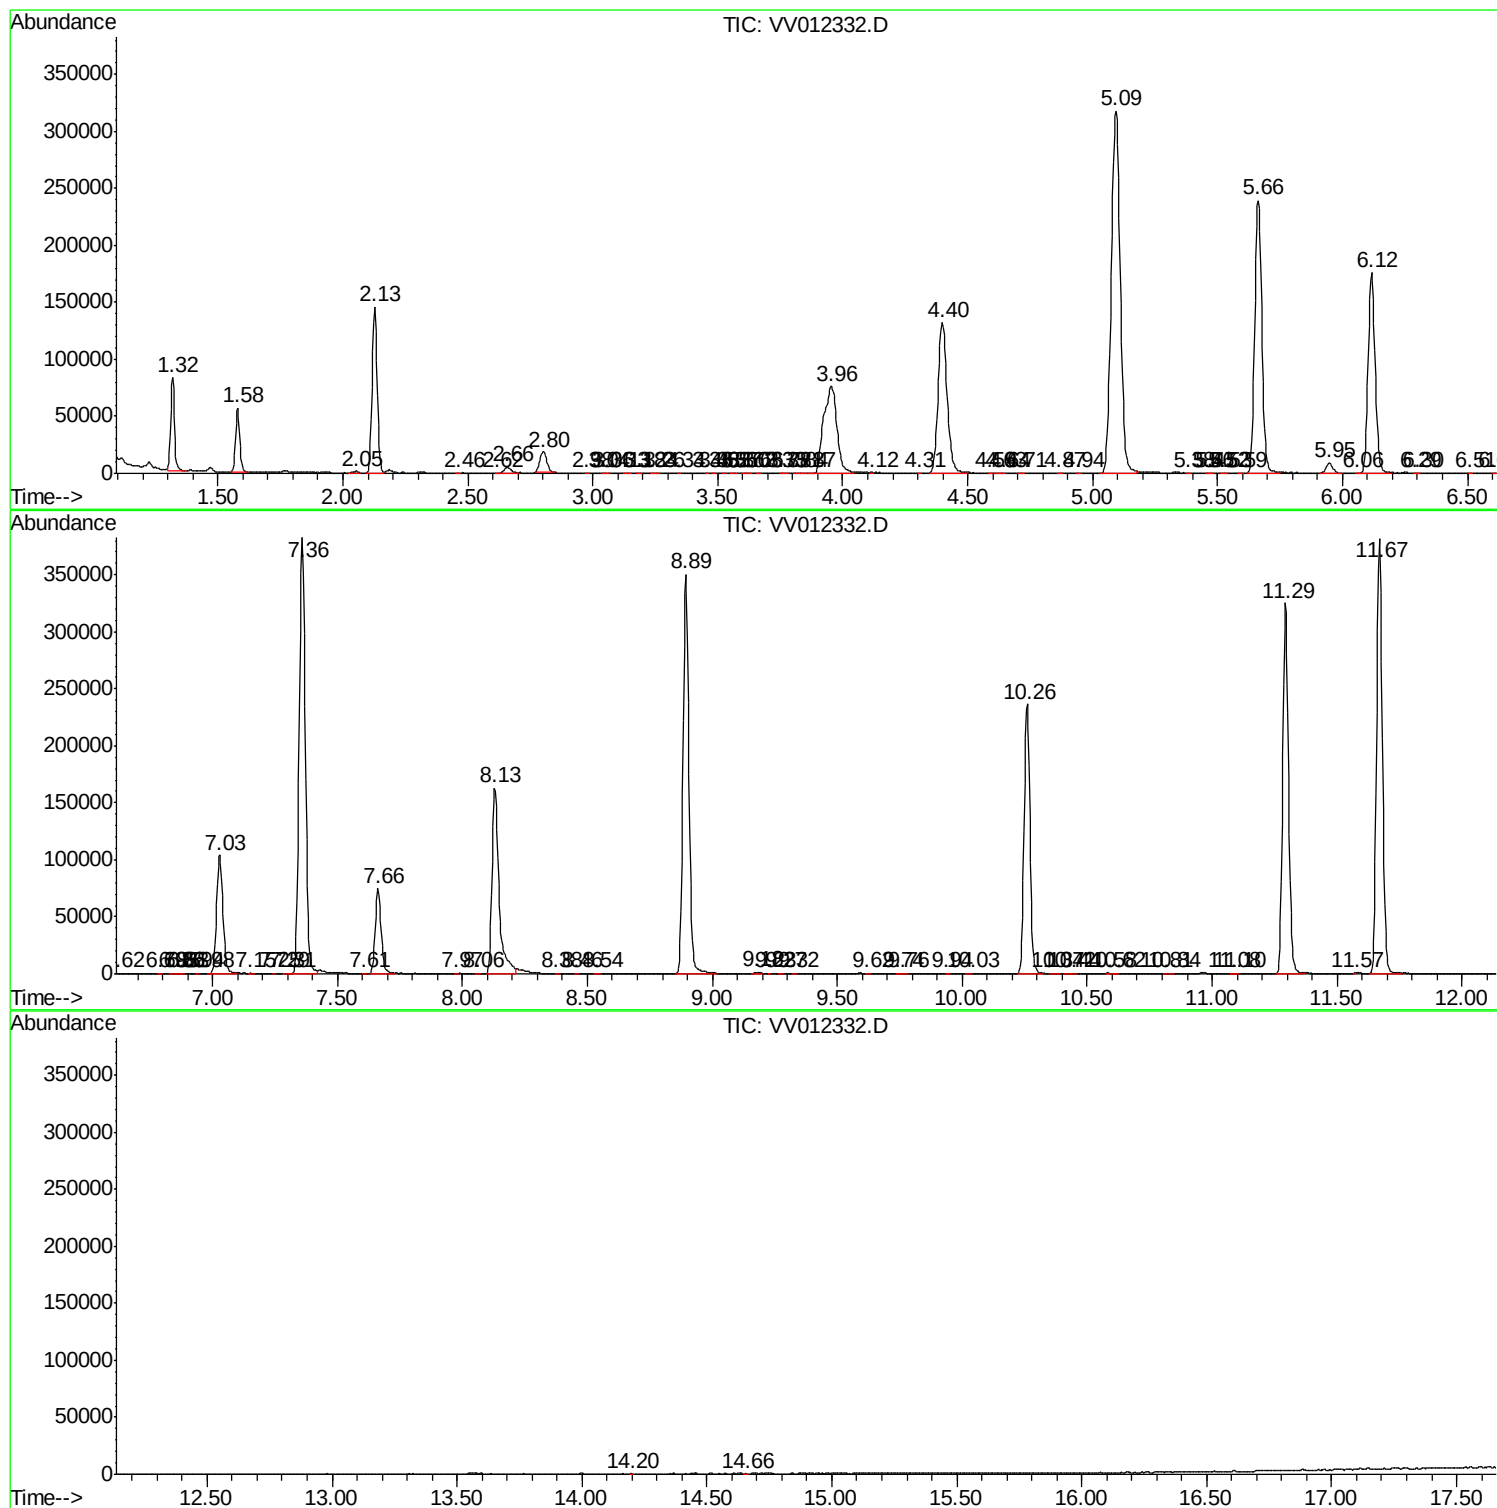

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012332.D
Acq On : 21 Aug 2019 23:12
Operator : SY/MD
Sample : K4454-11
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2C03

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012332.D
Acq On : 21 Aug 2019 23:12
Operator : SY/MD
Sample : K4454-11
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2C03

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
