

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012337.D
 Acq On : 22 Aug 2019 01:14
 Operator : SY/MD
 Sample : K4454-16
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2C12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	86	rVB	77075	81012	10.31%	1.382%
2	1.579	145	152	163	rVB	52985	62485	7.96%	1.066%
3	1.926	256	260	262	rBV	527	454	0.06%	0.008%
4	2.003	282	284	288	rVB	354	188	0.02%	0.003%
5	2.052	290	299	306	rBV4	1536	2204	0.28%	0.038%
6	2.129	312	323	337	rBV	144694	203610	25.92%	3.474%
7	2.229	350	354	356	rBV2	361	292	0.04%	0.005%
8	2.576	456	462	464	rBV2	305	290	0.04%	0.005%
9	2.733	508	511	514	rBV2	159	98	0.01%	0.002%
10	2.788	527	528	529	rBV2	247	74	0.01%	0.001%
11	2.872	552	554	557	rBV2	157	101	0.01%	0.002%
12	2.962	579	582	585	rBV	289	176	0.02%	0.003%
13	2.981	585	588	592	rBV2	238	141	0.02%	0.002%
14	3.007	594	596	599	rVB	195	84	0.01%	0.001%
15	3.023	599	601	602	rBV	158	81	0.01%	0.001%
16	3.071	613	616	618	rBV	259	130	0.02%	0.002%
17	3.119	629	631	633	rBV2	156	109	0.01%	0.002%
18	3.187	650	652	655	rVB	361	168	0.02%	0.003%
19	3.209	655	659	662	rBV2	353	299	0.04%	0.005%
20	3.328	693	696	698	rBV	137	81	0.01%	0.001%
21	3.376	709	711	714	rVB	165	93	0.01%	0.002%
22	3.418	722	724	729	rVB	185	96	0.01%	0.002%
23	3.454	732	735	736	rBV	146	105	0.01%	0.002%
24	3.489	743	746	747	rBV	270	158	0.02%	0.003%
25	3.569	769	771	774	rBV	201	103	0.01%	0.002%
26	3.650	793	796	797	rVB	253	98	0.01%	0.002%
27	3.659	797	799	802	rVB	177	77	0.01%	0.001%
28	3.708	811	814	816	rBV2	342	161	0.02%	0.003%
29	3.785	835	838	841	rVB	210	146	0.02%	0.002%
30	3.933	871	884	929	rBV4	44241	143471	18.27%	2.448%
31	4.196	964	966	969	rVB	261	138	0.02%	0.002%
32	4.212	969	971	973	rBV2	266	172	0.02%	0.003%
33	4.270	981	989	992	rBV3	363	503	0.06%	0.009%
34	4.318	1002	1004	1007	rBV2	275	153	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012337.D
 Acq On : 22 Aug 2019 01:14
 Operator : SY/MD
 Sample : K4454-16
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2C12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	4.341	1009	1011	1013	rVV	271	138	0.02%	0.002%
36	4.399	1013	1029	1059	rVV2	131653	329438	41.94%	5.621%
37	4.515	1063	1065	1069	rVB2	357	191	0.02%	0.003%
38	4.740	1131	1135	1138	rBV	186	164	0.02%	0.003%
39	4.788	1146	1150	1155	rBV2	213	253	0.03%	0.004%
40	5.010	1216	1219	1222	rBV	226	143	0.02%	0.002%
41	5.093	1227	1245	1268	rBV3	312128	785440	100.00%	13.402%
42	5.338	1319	1321	1323	rVB	343	121	0.02%	0.002%
43	5.466	1359	1361	1363	rBV2	146	85	0.01%	0.001%
44	5.505	1369	1373	1375	rVB2	303	188	0.02%	0.003%
45	5.534	1379	1382	1385	rBV	248	186	0.02%	0.003%
46	5.662	1408	1422	1447	rBV	249401	488119	62.15%	8.329%
47	5.949	1500	1511	1526	rVB3	8962	17393	2.21%	0.297%
48	6.039	1537	1539	1540	rBV	167	85	0.01%	0.001%
49	6.116	1549	1563	1581	rBV	172102	341705	43.50%	5.831%
50	6.325	1625	1628	1629	rBV	344	145	0.02%	0.002%
51	6.444	1663	1665	1668	rBV	219	138	0.02%	0.002%
52	6.537	1692	1694	1697	rBV2	166	117	0.01%	0.002%
53	6.601	1711	1714	1716	rVB	163	86	0.01%	0.001%
54	6.614	1716	1718	1720	rBV	178	122	0.02%	0.002%
55	6.653	1728	1730	1733	rBV2	293	200	0.03%	0.003%
56	6.701	1742	1745	1747	rBV	219	139	0.02%	0.002%
57	6.907	1807	1809	1813	rVB	200	82	0.01%	0.001%
58	7.029	1833	1847	1870	rBV	102600	179895	22.90%	3.070%
59	7.232	1907	1910	1912	rVB	291	126	0.02%	0.002%
60	7.248	1912	1915	1918	rBV	243	169	0.02%	0.003%
61	7.360	1936	1950	1968	rBV	377921	654198	83.29%	11.163%
62	7.579	2015	2018	2021	rBV2	417	325	0.04%	0.006%
63	7.662	2033	2044	2062	rBV2	72171	121156	15.43%	2.067%
64	7.820	2089	2093	2096	rBV	330	207	0.03%	0.004%
65	7.855	2100	2104	2108	rVB	170	150	0.02%	0.003%
66	7.891	2110	2115	2117	rBV2	218	218	0.03%	0.004%
67	7.968	2136	2139	2140	rBV2	228	148	0.02%	0.003%
68	8.129	2178	2189	2223	rBV2	167236	329006	41.89%	5.614%
69	8.318	2246	2248	2250	rBV	373	163	0.02%	0.003%
70	8.402	2272	2274	2276	rBV	259	113	0.01%	0.002%
71	8.457	2288	2291	2292	rBV	174	121	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082119\
 Data File : VV012337.D
 Acq On : 22 Aug 2019 01:14
 Operator : SY/MD
 Sample : K4454-16
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F2C12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	8.537	2314	2316	2318	rBV2	235	97	0.01%	0.002%
73	8.656	2351	2353	2357	rBV2	216	183	0.02%	0.003%
74	8.730	2375	2376	2381	rBV2	265	163	0.02%	0.003%
75	8.894	2414	2427	2456	rBV	359410	588910	74.98%	10.049%
76	9.055	2474	2477	2479	rVB	498	211	0.03%	0.004%
77	9.067	2479	2481	2482	rBV	271	134	0.02%	0.002%
78	9.103	2487	2492	2500	rBV3	393	570	0.07%	0.010%
79	9.151	2505	2507	2510	rBV2	172	104	0.01%	0.002%
80	9.257	2538	2540	2542	rBV	170	91	0.01%	0.002%
81	9.399	2581	2584	2589	rBV2	200	222	0.03%	0.004%
82	9.473	2604	2607	2611	rVB2	247	203	0.03%	0.003%
83	9.534	2623	2626	2629	rBV	183	138	0.02%	0.002%
84	9.566	2632	2636	2638	rBV2	169	116	0.01%	0.002%
85	9.672	2666	2669	2671	rBV	155	99	0.01%	0.002%
86	9.881	2730	2734	2738	rVB2	216	218	0.03%	0.004%
87	9.903	2738	2741	2742	rBV	218	131	0.02%	0.002%
88	10.006	2770	2773	2776	rBV2	168	148	0.02%	0.003%
89	10.260	2840	2852	2873	rBV	233367	368941	46.97%	6.295%
90	10.363	2880	2884	2887	rBV2	202	185	0.02%	0.003%
91	10.711	2988	2992	2995	rBV2	197	225	0.03%	0.004%
92	10.762	3003	3008	3011	rBV2	342	428	0.05%	0.007%
93	10.874	3041	3043	3045	rBV2	175	98	0.01%	0.002%
94	10.971	3069	3073	3076	rBV2	186	181	0.02%	0.003%
95	11.292	3161	3173	3192	rBV	333826	536824	68.35%	9.160%
96	11.444	3217	3220	3221	rBV2	234	116	0.01%	0.002%
97	11.669	3277	3290	3311	rBV	379828	612965	78.04%	10.459%
98	11.894	3358	3360	3363	rBV	241	193	0.02%	0.003%
99	12.289	3480	3483	3486	rBV	269	218	0.03%	0.004%
100	12.328	3492	3495	3498	rBV	227	211	0.03%	0.004%


Sum of corrected areas: 5860547

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082119\
Data File : VV012337.D
Acq On : 22 Aug 2019 01:14
Operator : SY/MD
Sample : K4454-16
Misc : 5mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F2C12

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

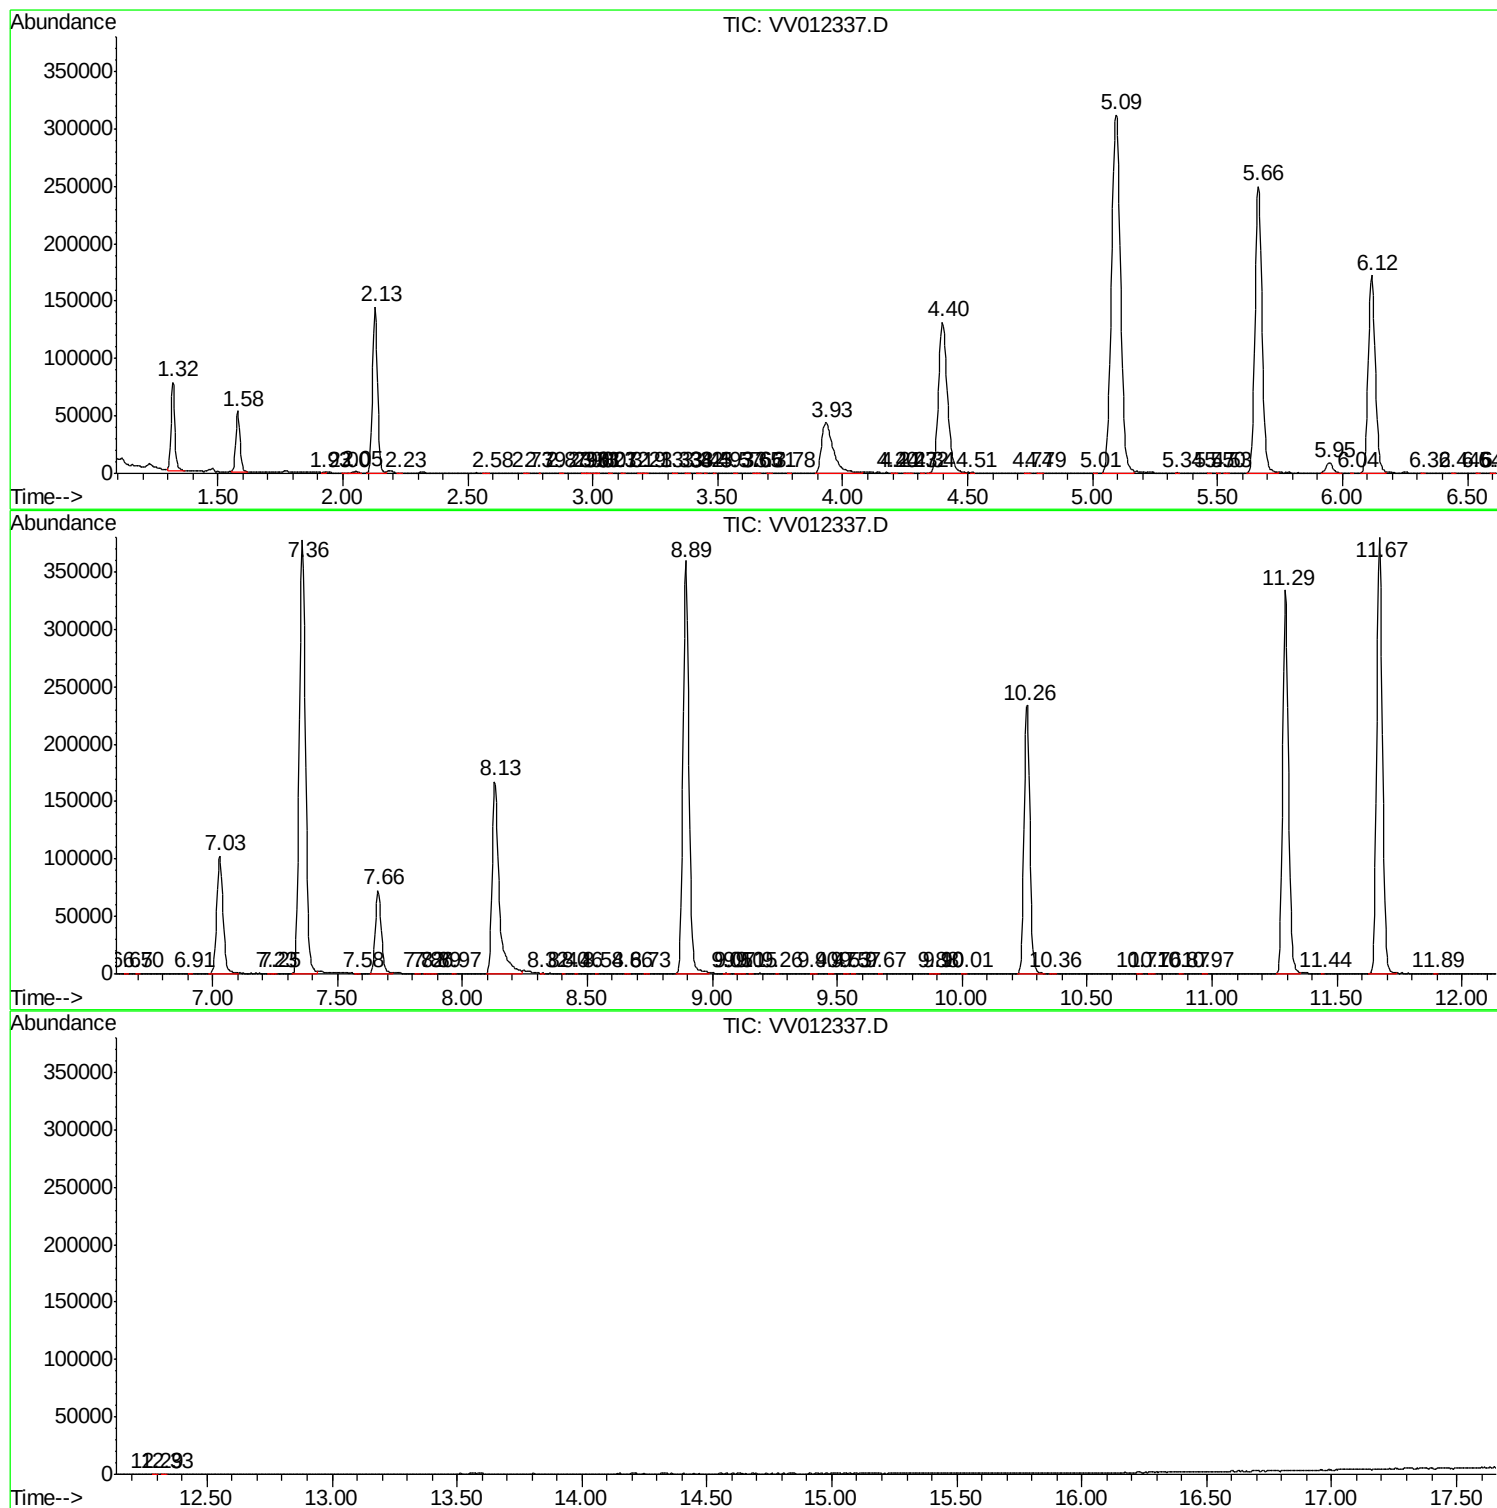

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012337.D
Acq On : 22 Aug 2019 01:14
Operator : SY/MD
Sample : K4454-16
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2C12

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082119\
Data File : VV012337.D
Acq On : 22 Aug 2019 01:14
Operator : SY/MD
Sample : K4454-16
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F2C12

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc