


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082120\
 Data File : VV018071.D
 Acq On : 21 Aug 2020 09:16
 Operator : SY/MD
 Sample : BFB79
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB79

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Mon Aug 24 12:58:36 2020

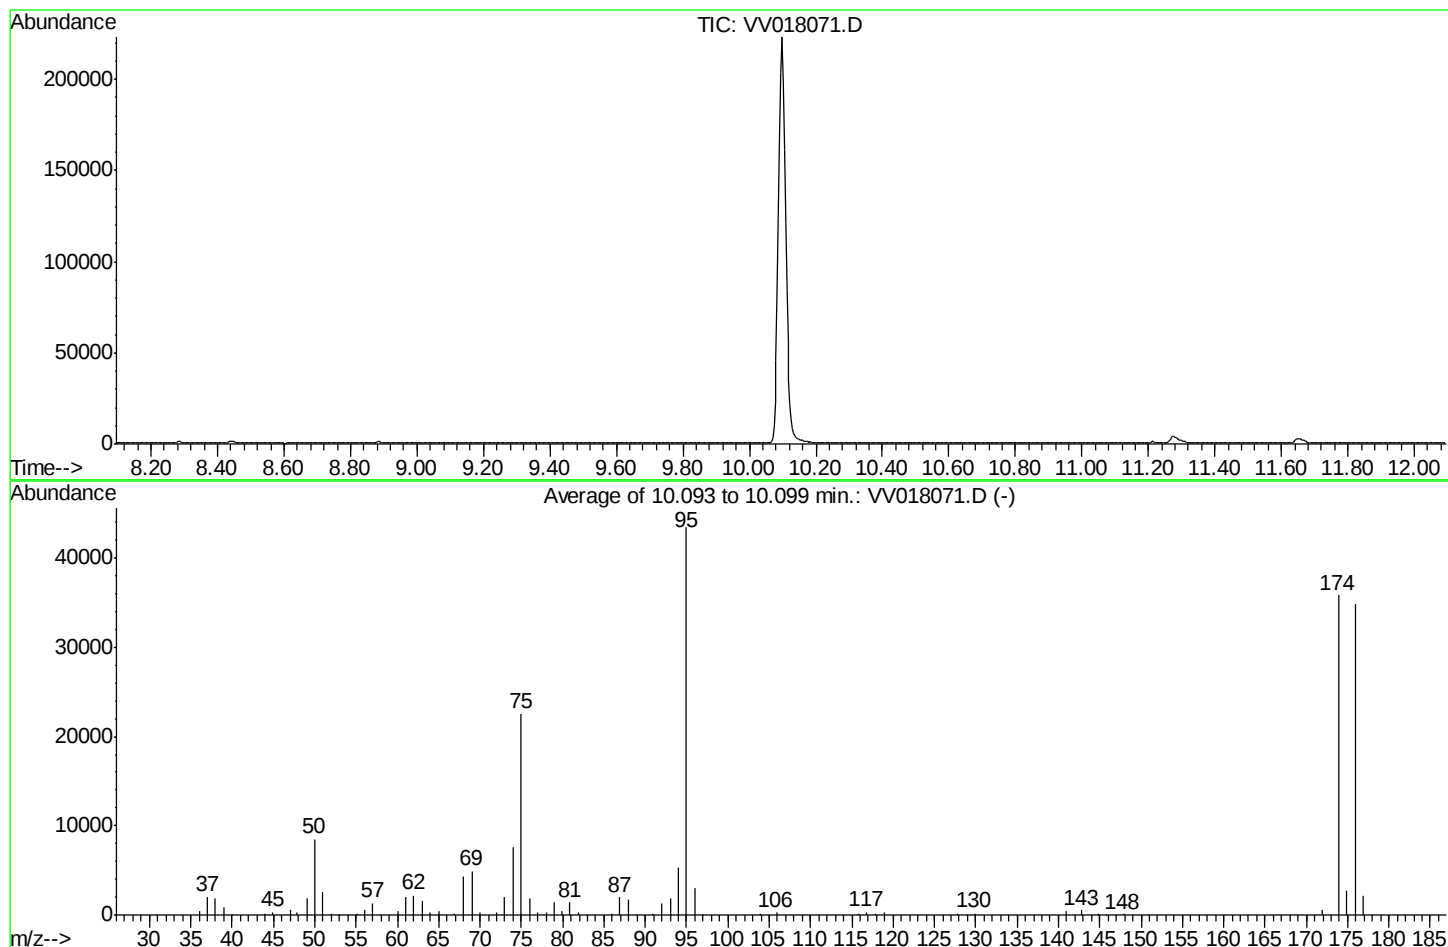

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	8471	PASS
75	95	30	80	51.9	22552	PASS
95	95	100	100	100.0	43432	PASS
96	95	5	9	6.8	2969	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.4	35792	PASS
175	174	5	9	7.8	2784	PASS
176	174	95	101	97.4	34877	PASS
177	176	5	9	6.3	2214	PASS

m/z	Abundance
36.00	391.0
37.00	2032.0
38.00	1855.0
39.00	914.0
39.90	185.0
43.90	503.0
45.00	309.0
47.00	560.0
47.90	258.0
49.00	1816.0
50.00	8152.0
51.00	2550.0
51.90	141.0
52.90	103.0
54.90	110.0
56.00	569.0
57.00	1273.0
60.00	467.0
61.00	1940.0
62.00	2201.0
63.00	1606.0
64.00	268.0
65.00	429.0
66.80	151.0
68.00	4192.0
69.00	4623.0
70.00	349.0
72.00	221.0
73.00	1919.0
74.00	7232.0
75.00	21592.0
76.00	1802.0
76.90	307.0
78.10	211.0
78.90	1302.0
79.90	458.0
80.90	1339.0
81.90	327.0
87.00	1983.0
87.90	1765.0
90.90	186.0
91.90	1284.0
93.00	1793.0
94.00	5022.0
95.00	41184.0
96.00	2983.0
103.90	186.0
105.90	224.0
115.80	144.0
116.80	318.0
117.90	180.0
118.90	247.0
127.80	173.0
129.90	168.0
140.90	459.0
142.80	540.0
144.80	146.0
171.90	552.0
173.90	32808.0
174.90	2576.0
175.90	32144.0
177.00	2166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	425.0
37.00	2147.0
38.00	1931.0
39.00	912.0
39.90	186.0
43.90	471.0
44.90	344.0
47.00	629.0
47.90	291.0
49.00	1987.0
50.00	8718.0
51.00	2659.0
51.90	131.0
53.00	107.0
55.10	120.0
56.00	666.0
57.00	1338.0
60.00	490.0
61.00	2072.0
62.00	2277.0
63.00	1693.0
64.00	294.0
65.00	440.0
66.80	140.0
68.00	4495.0
69.00	5122.0
70.00	338.0
72.00	256.0
73.00	2137.0
74.00	7737.0
75.00	23392.0
76.00	1899.0
77.00	332.0
78.10	244.0
78.90	1504.0
79.90	505.0
80.90	1481.0
81.90	367.0
85.90	118.0
86.90	2023.0
88.00	1819.0
90.90	203.0
91.90	1413.0
93.00	1960.0
94.00	5484.0
95.00	44752.0
96.00	3066.0
97.00	103.0
103.90	192.0
105.90	250.0
115.80	163.0
116.80	330.0
117.90	206.0
118.90	291.0
127.80	192.0
129.90	209.0
140.90	489.0
142.90	584.0
144.80	192.0
147.80	125.0
171.90	568.0
173.90	36968.0
174.90	2916.0
175.90	36128.0
177.00	2275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

m/z	Abundance
36.00	396.0
37.00	2063.0
38.00	1840.0
39.00	828.0
40.00	200.0
44.00	442.0
44.90	346.0
47.00	601.0
47.90	303.0
49.00	1951.0
50.00	8545.0
51.00	2476.0
52.00	115.0
55.10	117.0
56.00	692.0
57.00	1274.0
60.00	476.0
61.00	2119.0
62.00	2111.0
63.00	1643.0
64.00	309.0
65.00	439.0
66.90	141.0
68.00	4377.0
69.00	4960.0
69.90	318.0
71.90	269.0
73.00	2073.0
74.00	7645.0
75.00	22672.0
76.00	1843.0
77.00	331.0
78.10	220.0
78.90	1536.0
79.90	498.0
80.90	1425.0
81.90	338.0
85.90	143.0
86.90	1965.0
88.00	1760.0
90.90	171.0
92.00	1377.0
93.00	1985.0
94.00	5438.0
95.00	44360.0
96.00	2859.0
103.80	195.0
105.90	234.0
115.80	163.0
116.80	285.0
117.90	194.0
118.90	286.0
127.80	181.0
128.90	115.0
129.90	211.0
140.90	506.0
142.90	573.0
144.90	225.0
145.80	101.0
147.90	133.0
171.90	519.0
173.90	37600.0
174.90	2860.0
175.90	36360.0
176.90	2203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79

Scan 2790 (10.061 min): VV018071.D
BFB79

m/z	Abundance
39.90	175.0
44.00	361.0

Instrument :
MSVOA_V
ClientSampleId :
BFB79