

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082219\
 Data File : VV012349.D
 Acq On : 22 Aug 2019 15:53
 Operator : SY/MD
 Sample : K4481-08
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COXM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.579	146	152	164	rVB	42130	50271	7.70%	0.969%
2	1.769	203	211	222	rVB	36417	46870	7.18%	0.904%
3	1.965	270	272	273	rBV	251	95	0.01%	0.002%
4	2.000	280	283	285	rBB	184	120	0.02%	0.002%
5	2.029	289	292	293	rBV	145	102	0.02%	0.002%
6	2.129	313	323	335	rBV	112392	157037	24.05%	3.028%
7	2.245	357	359	362	rBB	144	98	0.02%	0.002%
8	2.270	365	367	369	rBV	280	158	0.02%	0.003%
9	2.344	389	390	395	rBV2	288	209	0.03%	0.004%
10	2.537	447	450	453	rBB2	442	218	0.03%	0.004%
11	2.553	453	455	457	rBB	224	104	0.02%	0.002%
12	2.579	460	463	465	rBB	257	121	0.02%	0.002%
13	2.608	470	472	475	rBV	133	115	0.02%	0.002%
14	2.688	494	497	501	rBB	125	108	0.02%	0.002%
15	2.714	502	505	508	rBV	277	177	0.03%	0.003%
16	2.778	520	525	528	rBB	177	173	0.03%	0.003%
17	2.801	529	532	535	rBB	131	112	0.02%	0.002%
18	2.823	535	539	545	rBB	173	249	0.04%	0.005%
19	2.907	563	565	570	rBB	280	206	0.03%	0.004%
20	2.933	570	573	575	rBB	151	103	0.02%	0.002%
21	2.965	580	583	585	rBV	130	118	0.02%	0.002%
22	3.061	606	613	616	rBV	296	346	0.05%	0.007%
23	3.087	619	621	623	rBV	266	162	0.02%	0.003%
24	3.158	638	643	646	rBV	259	263	0.04%	0.005%
25	3.222	659	663	666	rBB2	279	182	0.03%	0.004%
26	3.254	669	673	677	rBB	179	170	0.03%	0.003%
27	3.277	678	680	686	rBB	251	251	0.04%	0.005%
28	3.306	687	689	692	rBB	189	120	0.02%	0.002%
29	3.354	699	704	706	rBV	202	215	0.03%	0.004%
30	3.434	726	729	734	rBV	131	185	0.03%	0.004%
31	3.518	753	755	758	rVV	217	102	0.02%	0.002%
32	3.817	845	848	852	rBV	216	222	0.03%	0.004%
33	3.923	870	881	914	rBV	46076	130564	19.99%	2.518%
34	4.296	994	997	1001	rBB3	477	372	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082219\
 Data File : VV012349.D
 Acq On : 22 Aug 2019 15:53
 Operator : SY/MD
 Sample : K4481-08
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

35	4.328	1001	1007	1010	rBV2	422	428	0.07%	0.008%
36	4.614	1094	1096	1098	rBV	150	102	0.02%	0.002%
37	4.746	1133	1137	1139	rBB	133	92	0.01%	0.002%
38	4.775	1144	1146	1149	rBB	130	91	0.01%	0.002%
39	4.862	1168	1173	1174	rBV	696	456	0.07%	0.009%
40	4.933	1189	1195	1198	rBV	261	223	0.03%	0.004%
41	5.093	1228	1245	1266	rBV2	260033	653057	100.00%	12.594%
42	5.489	1365	1368	1369	rBV	168	110	0.02%	0.002%
43	5.576	1392	1395	1399	rBB	172	160	0.02%	0.003%
44	5.598	1399	1402	1404	rBB	153	99	0.02%	0.002%
45	5.662	1407	1422	1439	rBV	203257	395865	60.62%	7.634%
46	5.958	1500	1514	1533	rBV2	199861	389579	59.65%	7.513%
47	6.116	1549	1563	1580	rBV2	142550	284702	43.60%	5.491%
48	6.244	1600	1603	1604	rBV2	521	260	0.04%	0.005%
49	6.396	1647	1650	1653	rBB	181	145	0.02%	0.003%
50	6.412	1653	1655	1657	rBV	148	106	0.02%	0.002%
51	6.479	1673	1676	1678	rBB	165	111	0.02%	0.002%
52	6.502	1681	1683	1685	rBV	233	116	0.02%	0.002%
53	6.588	1704	1710	1713	rBV	174	251	0.04%	0.005%
54	6.633	1721	1724	1726	rBV	270	173	0.03%	0.003%
55	6.740	1753	1757	1759	rBV	178	162	0.02%	0.003%
56	6.826	1780	1784	1785	rBV	145	131	0.02%	0.003%
57	6.859	1789	1794	1801	rBB	177	302	0.05%	0.006%
58	6.936	1812	1818	1821	rBV	194	271	0.04%	0.005%
59	7.029	1834	1847	1869	rBV	89353	157018	24.04%	3.028%
60	7.302	1928	1932	1933	rBV	152	129	0.02%	0.002%
61	7.360	1937	1950	1968	rBV	312722	542049	83.00%	10.454%
62	7.662	2033	2044	2065	rBV	63903	105876	16.21%	2.042%
63	7.894	2114	2116	2118	rBV	145	101	0.02%	0.002%
64	8.019	2143	2155	2172	rBV	142517	240868	36.88%	4.645%
65	8.129	2179	2189	2220	rBV2	135756	269233	41.23%	5.192%
66	8.328	2250	2251	2253	rBV	245	97	0.01%	0.002%
67	8.392	2268	2271	2273	rBV2	280	199	0.03%	0.004%
68	8.444	2283	2287	2288	rBV	191	161	0.02%	0.003%
69	8.511	2305	2308	2310	rBV	150	129	0.02%	0.002%
70	8.646	2347	2350	2352	rBV	317	195	0.03%	0.004%
71	8.698	2364	2366	2368	rBB	243	110	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082219\
 Data File : VV012349.D
 Acq On : 22 Aug 2019 15:53
 Operator : SY/MD
 Sample : K4481-08
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
 Title : VOC Analysis

72	8.746	2378	2381	2385	rBV	134	139	0.02%	0.003%
73	8.794	2393	2396	2402	rBV	329	346	0.05%	0.007%
74	8.894	2415	2427	2446	rBV	297857	483496	74.04%	9.324%
75	9.276	2543	2546	2548	rBV	258	127	0.02%	0.002%
76	9.334	2560	2564	2568	rBV2	299	330	0.05%	0.006%
77	9.508	2613	2618	2621	rBV	174	209	0.03%	0.004%
78	9.566	2633	2636	2639	rBB	147	122	0.02%	0.002%
79	9.585	2639	2642	2643	rBV	260	165	0.03%	0.003%
80	9.804	2707	2710	2713	rBV	289	260	0.04%	0.005%
81	9.907	2738	2742	2744	rBV	309	292	0.04%	0.006%
82	10.109	2801	2805	2809	rBV2	289	317	0.05%	0.006%
83	10.209	2834	2836	2840	rBV	308	231	0.04%	0.004%
84	10.260	2840	2852	2873	rVV	199151	317002	48.54%	6.113%
85	10.592	2951	2955	2958	rBV2	328	311	0.05%	0.006%
86	10.633	2965	2968	2970	rBV2	244	175	0.03%	0.003%
87	10.669	2977	2979	2982	rBV	252	174	0.03%	0.003%
88	10.772	3009	3011	3014	rBV2	282	151	0.02%	0.003%
89	10.919	3053	3057	3060	rBB2	281	289	0.04%	0.006%
90	10.939	3060	3063	3065	rBV	273	188	0.03%	0.004%
91	11.112	3115	3117	3118	rBV	241	117	0.02%	0.002%
92	11.141	3121	3126	3130	rBV2	310	379	0.06%	0.007%
93	11.209	3144	3147	3149	rBV2	346	248	0.04%	0.005%
94	11.251	3157	3160	3162	rBV	234	153	0.02%	0.003%
95	11.292	3162	3173	3191	rVV	264544	429300	65.74%	8.279%
96	11.485	3230	3233	3234	rBV	155	104	0.02%	0.002%
97	11.669	3278	3290	3309	rBV	318467	517110	79.18%	9.973%
98	12.447	3528	3532	3535	rBV2	293	268	0.04%	0.005%
99	12.765	3629	3631	3634	rBV2	251	117	0.02%	0.002%
100	13.450	3841	3844	3845	rBV	286	119	0.02%	0.002%


Sum of corrected areas: 5185314

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082219\
Data File : VV012349.D
Acq On : 22 Aug 2019 15:53
Operator : SY/MD
Sample : K4481-08
Misc : 5mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COXM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

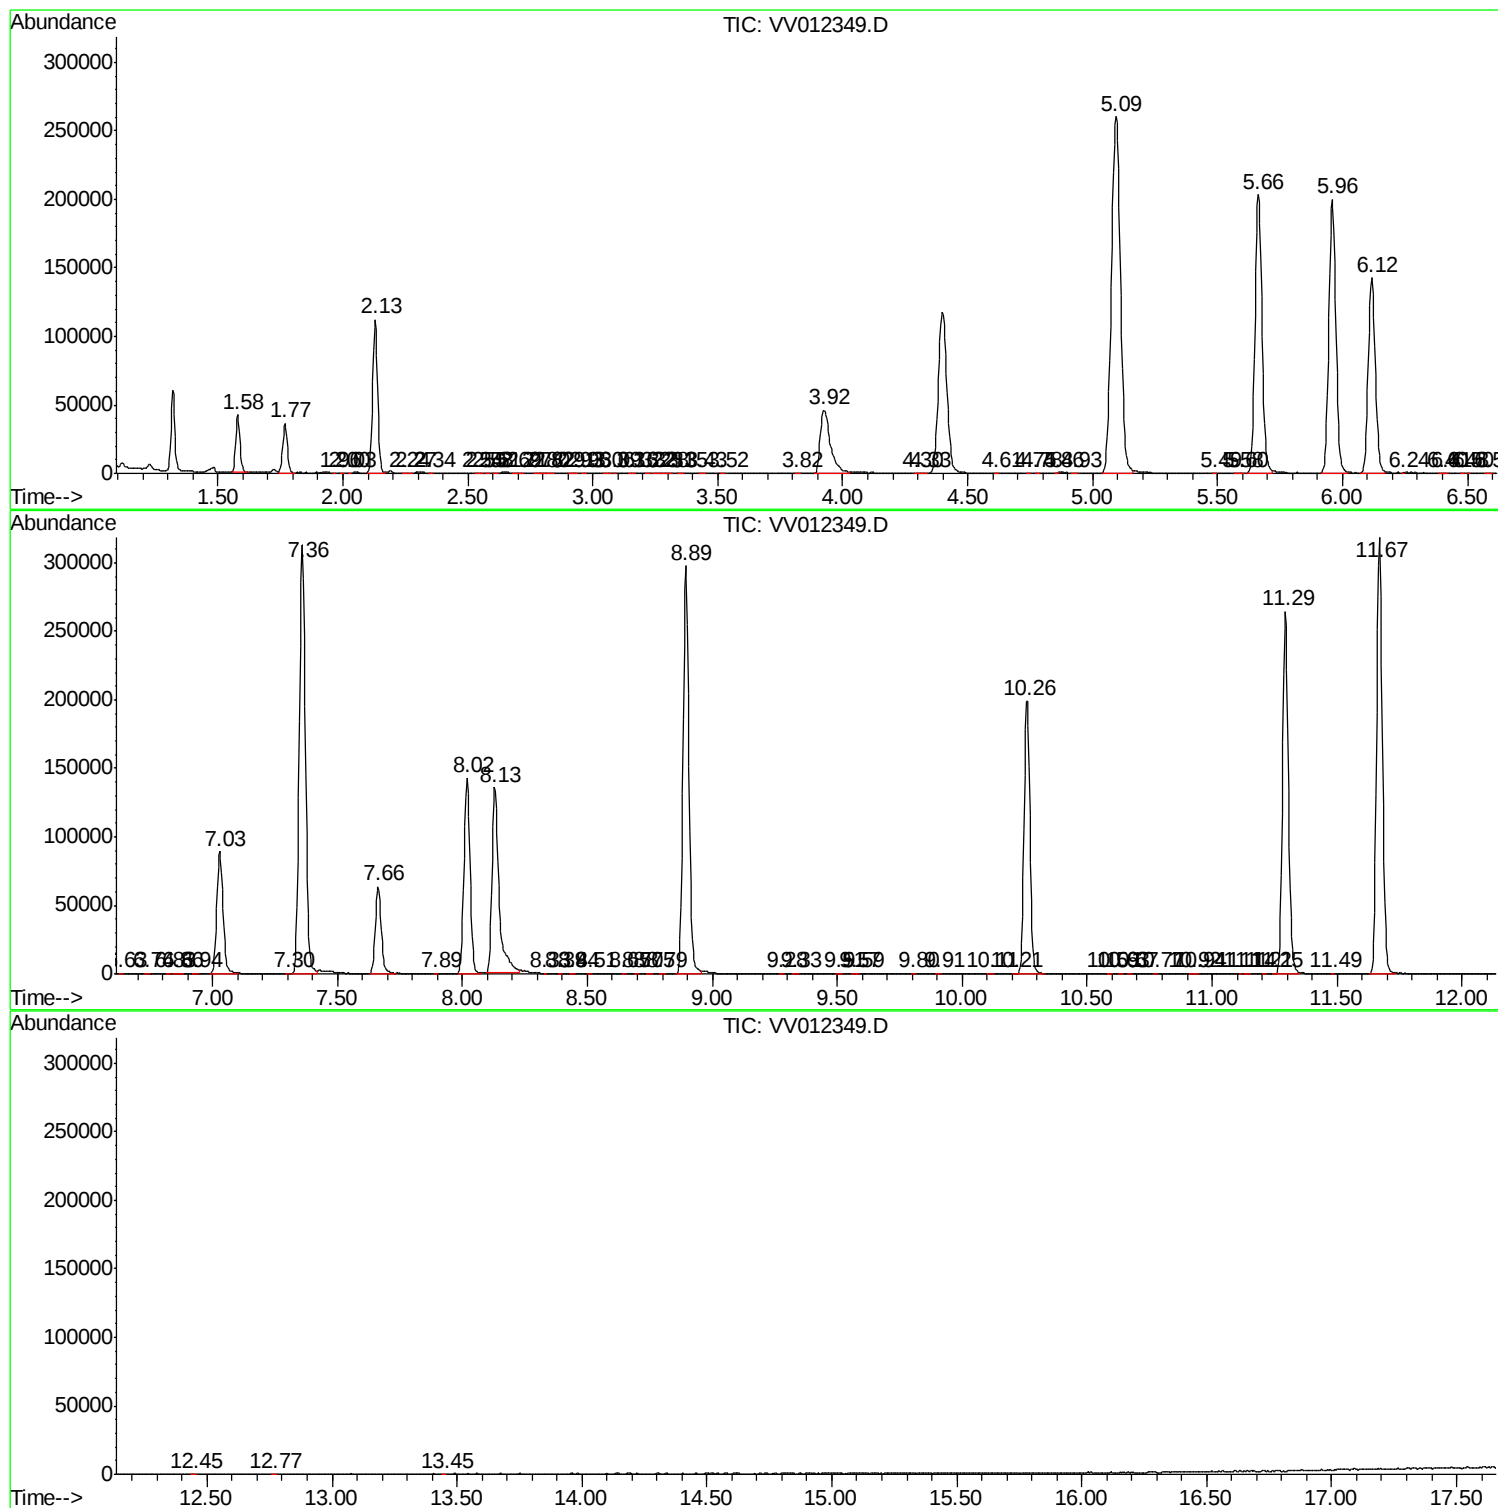

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV082219\
Data File : VV012349.D
Acq On : 22 Aug 2019 15:53
Operator : SY/MD
Sample : K4481-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV082219\
Data File : VV012349.D
Acq On : 22 Aug 2019 15:53
Operator : SY/MD
Sample : K4481-08
Misc : 5mL/MSV0A_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0XM6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM082119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc