


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082219\
Data File : VV012339.D
Acq On : 22 Aug 2019 10:30
Operator : SY/MD
Sample : BFB67
Misc : 5mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082119WMA.M
Title : VOC Analysis
Last Update : Fri Aug 23 06:55:48 2019

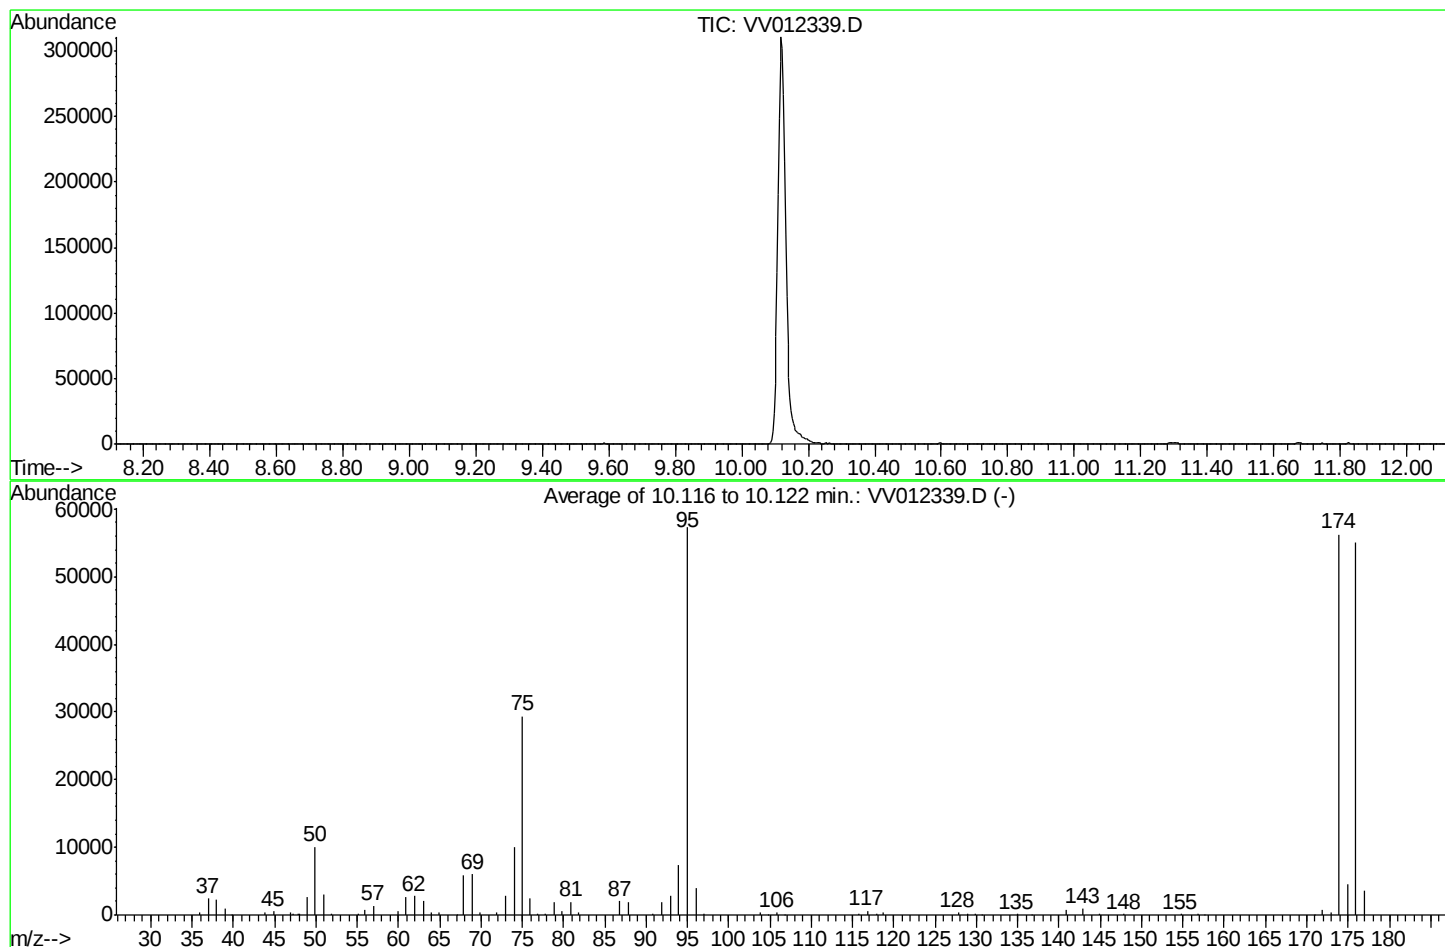

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	10032	PASS
75	95	30	80	51.2	29328	PASS
95	95	100	100	100.0	57280	PASS
96	95	5	9	6.9	3965	PASS
173	174	0.00	2	0.5	304	PASS
174	95	50	120	98.2	56221	PASS
175	174	5	9	8.0	4470	PASS
176	174	95	101	97.9	55066	PASS
177	176	5	9	6.5	3577	PASS

m/z	Abundance
35.80	447.0
36.90	2361.0
38.00	2159.0
39.00	1018.0
39.80	149.0
43.90	484.0
44.90	534.0
46.90	423.0
47.80	307.0
48.90	2617.0
49.90	10016.0
51.00	3052.0
51.90	129.0
55.10	224.0
55.90	840.0
56.90	1449.0
60.00	668.0
60.90	2575.0
61.90	2861.0
63.00	1973.0
63.90	348.0
65.00	563.0
67.90	5507.0
69.00	5902.0
69.90	379.0
71.90	334.0
72.90	2591.0
74.00	10060.0
75.00	28592.0
75.90	2500.0
77.00	265.0
77.80	178.0
78.90	1832.0
79.80	584.0
80.90	1847.0
81.80	324.0
86.80	1928.0
88.00	1754.0
90.80	248.0
91.90	1897.0
93.00	2925.0
94.00	7514.0
95.00	55064.0
96.00	3910.0
96.90	159.0
103.80	280.0
105.80	326.0
106.80	128.0
115.90	236.0
116.80	514.0
118.00	136.0
118.80	384.0
127.80	230.0
128.90	160.0
129.80	225.0
135.00	128.0
136.70	120.0
140.90	768.0
143.00	775.0
145.00	253.0
147.90	194.0
154.90	124.0
156.90	156.0
170.90	119.0
171.90	709.0
173.00	914.0
173.90	53248.0
174.90	4162.0
175.90	52864.0
176.90	3519.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.80	450.0
36.90	2505.0
38.00	2385.0
39.00	985.0
39.90	171.0
43.90	469.0
44.90	506.0
46.80	468.0
48.00	329.0
49.00	2718.0
49.90	10339.0
51.00	3255.0
51.90	151.0
55.10	250.0
55.90	837.0
56.90	1398.0
60.00	597.0
60.90	2650.0
62.00	2837.0
63.00	2076.0
64.00	396.0
65.00	483.0
67.10	124.0
67.90	6010.0
68.90	6197.0
69.90	350.0
71.90	319.0
72.90	2947.0
74.00	10421.0
75.00	30160.0
75.90	2487.0
76.80	290.0
77.80	234.0
78.90	2048.0
79.90	550.0
80.90	1951.0
81.80	376.0
86.80	2081.0
87.90	1873.0
90.80	261.0
91.90	1952.0
93.00	3008.0
94.00	7665.0
95.00	59224.0
96.00	4142.0
96.90	126.0
103.80	311.0
104.80	111.0
105.90	323.0
106.80	116.0
115.80	242.0
116.80	601.0
117.90	165.0
118.80	401.0
127.80	291.0
129.00	187.0
129.80	204.0
130.70	105.0
135.00	121.0
136.70	112.0
140.80	774.0
142.90	905.0
145.00	262.0
147.90	170.0
154.70	147.0
156.90	157.0
157.60	104.0
171.90	850.0
173.90	58000.0
174.90	4657.0
175.90	56600.0
176.90	3726.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.90	458.0
37.00	2474.0
38.00	2344.0
39.00	941.0
39.90	215.0
43.90	389.0
44.90	405.0
46.80	409.0
47.30	320.0
48.00	370.0
49.00	2445.0
49.90	9743.0
51.00	3070.0
51.90	152.0
55.10	204.0
55.90	775.0
57.00	1308.0
60.00	459.0
60.90	2605.0
62.00	2695.0
63.00	1978.0
64.00	359.0
64.90	382.0
67.90	5880.0
68.90	6055.0
69.90	342.0
71.90	338.0
72.90	2820.0
74.00	9663.0
75.00	29232.0
75.90	2298.0
76.80	267.0
77.80	257.0
78.90	2012.0
79.90	509.0
80.90	1933.0
81.80	412.0
86.80	2152.0
87.80	1936.0
90.80	256.0
92.00	1866.0
93.00	2758.0
93.90	7064.0
95.00	57552.0
96.00	3845.0
97.00	113.0
103.90	313.0
104.80	132.0
105.90	263.0
115.70	238.0
116.80	619.0
117.80	200.0
118.70	405.0
127.80	357.0
129.00	162.0
129.80	226.0
130.70	113.0
134.80	140.0
140.80	711.0
142.80	1032.0
144.90	209.0
147.90	138.0
154.80	203.0
156.90	154.0
171.90	883.0
173.90	57416.0
174.90	4592.0
175.90	55736.0
176.90	3487.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Scan 2796 (10.080 min): VV012339.D
BFB67

m/z	Abundance
39.80	175.0
43.90	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67