

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027459.D
 Acq On : 22 Aug 2022 11:40
 Operator : SY/MD
 Sample : N4268-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8

Quant Time: Aug 23 03:11:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 23 03:03:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	118156	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	117653	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50450	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	40092	4.768	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.400%
7) Chloroethane-d5	1.568	69	39003	6.337	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	126.800%
11) 1,1-Dichloroethene-d2	2.105	63	73096	3.728	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.600%
20) 2-Butanone-d5	3.899	46	37321	35.662	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	71.320%
24) Chloroform-d	4.349	84	83120	4.943	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.031	65	36953	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.047	84	153899	4.723	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
36) 1,2-Dichloropropane-d6	6.069	67	47178	4.979	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.600%
41) Toluene-d8	7.313	98	123189	4.187	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.800%
43) trans-1,3-Dichloroprop...	7.625	79	15152	4.671	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.400%
46) 2-Hexanone-d5	8.091	63	43257	40.508	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30470	5.050	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	39345	5.261	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.200%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	5653	0.419	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027459.D
Acq On : 22 Aug 2022 11:40
Operator : SY/MD
Sample : N4268-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8

Quant Time: Aug 23 03:11:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 23 03:03:07 2022
Response via : Initial Calibration

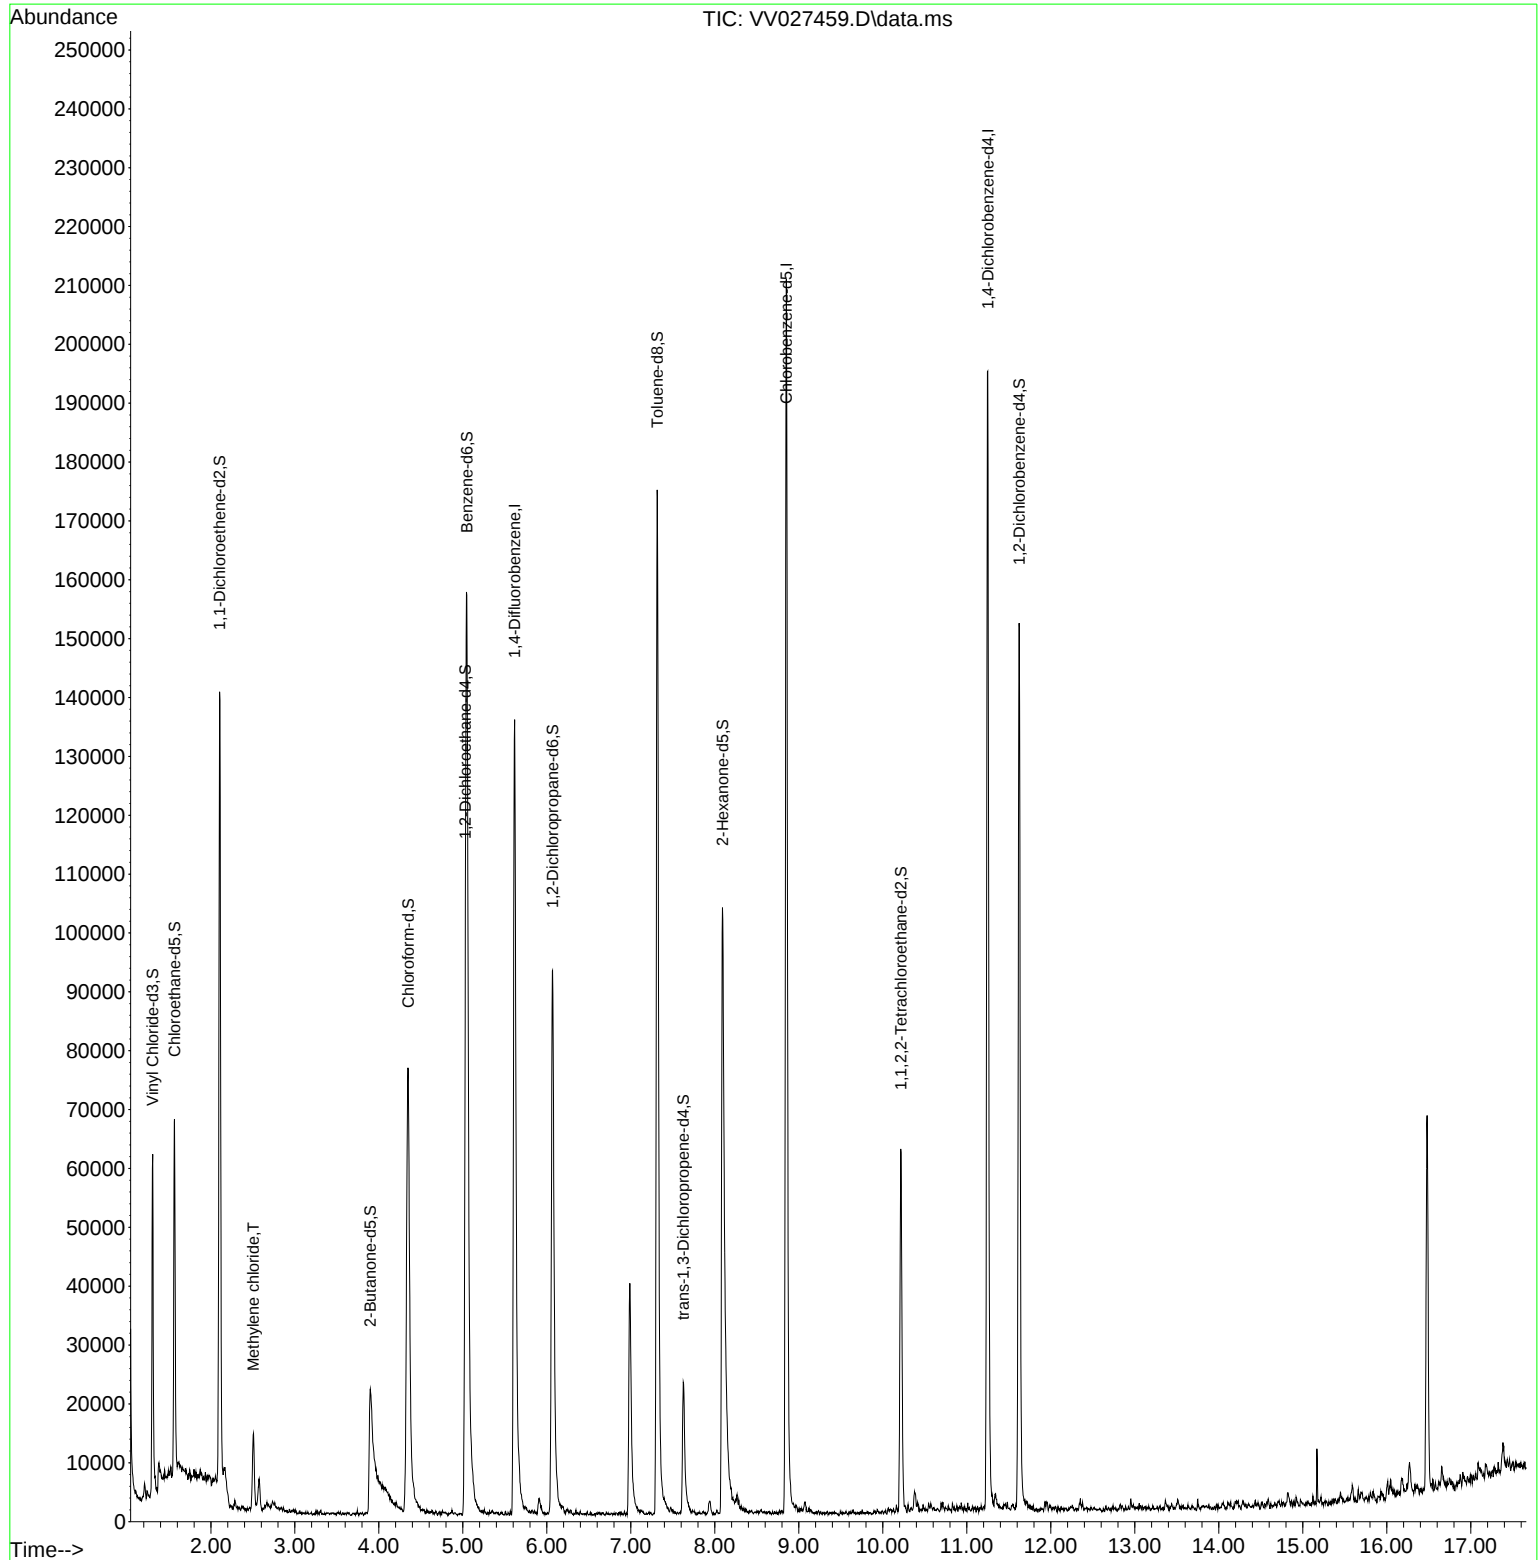

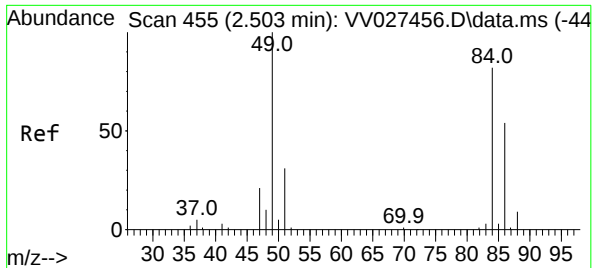

#16
Methylene chloride
Concen: 0.419 ug/L
RT: 2.507 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV027459.D
Acq: 22 Aug 2022 11:40

Instrument :
MSVOA_V
ClientSampleId :
C0AB8

Tgt Ion: 84	Resp:	5653
Ion	Ratio	Lower Upper
84	100	
86	55.6	44.0 81.6
49	118.6	89.4 166.0

