

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027460.D
 Acq On : 22 Aug 2022 12:04
 Operator : SY/MD
 Sample : N4252-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9C2

Quant Time: Aug 23 03:11:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 23 03:03:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	117102	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	118984	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51095	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	39985	4.798	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.000%
7) Chloroethane-d5	1.568	69	40317	6.610	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	132.200%#
11) 1,1-Dichloroethene-d2	2.105	63	70908	3.649	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.000%
20) 2-Butanone-d5	3.896	46	62352	60.117	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.240%
24) Chloroform-d	4.346	84	82761	4.966	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.034	65	35909	4.981	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%
32) Benzene-d6	5.050	84	154335	4.683	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.069	67	47456	4.953	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.317	98	125037	4.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%
43) trans-1,3-Dichloroprop...	7.625	79	14971	4.563	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.092	63	49368	45.714	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	29203	4.786	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	40591	5.359	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%
Target Compounds						Qvalue
3) Chloromethane	1.240	50	6966	0.642	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027460.D
Acq On : 22 Aug 2022 12:04
Operator : SY/MD
Sample : N4252-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C2


Quant Time: Aug 23 03:11:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 23 03:03:07 2022
Response via : Initial Calibration

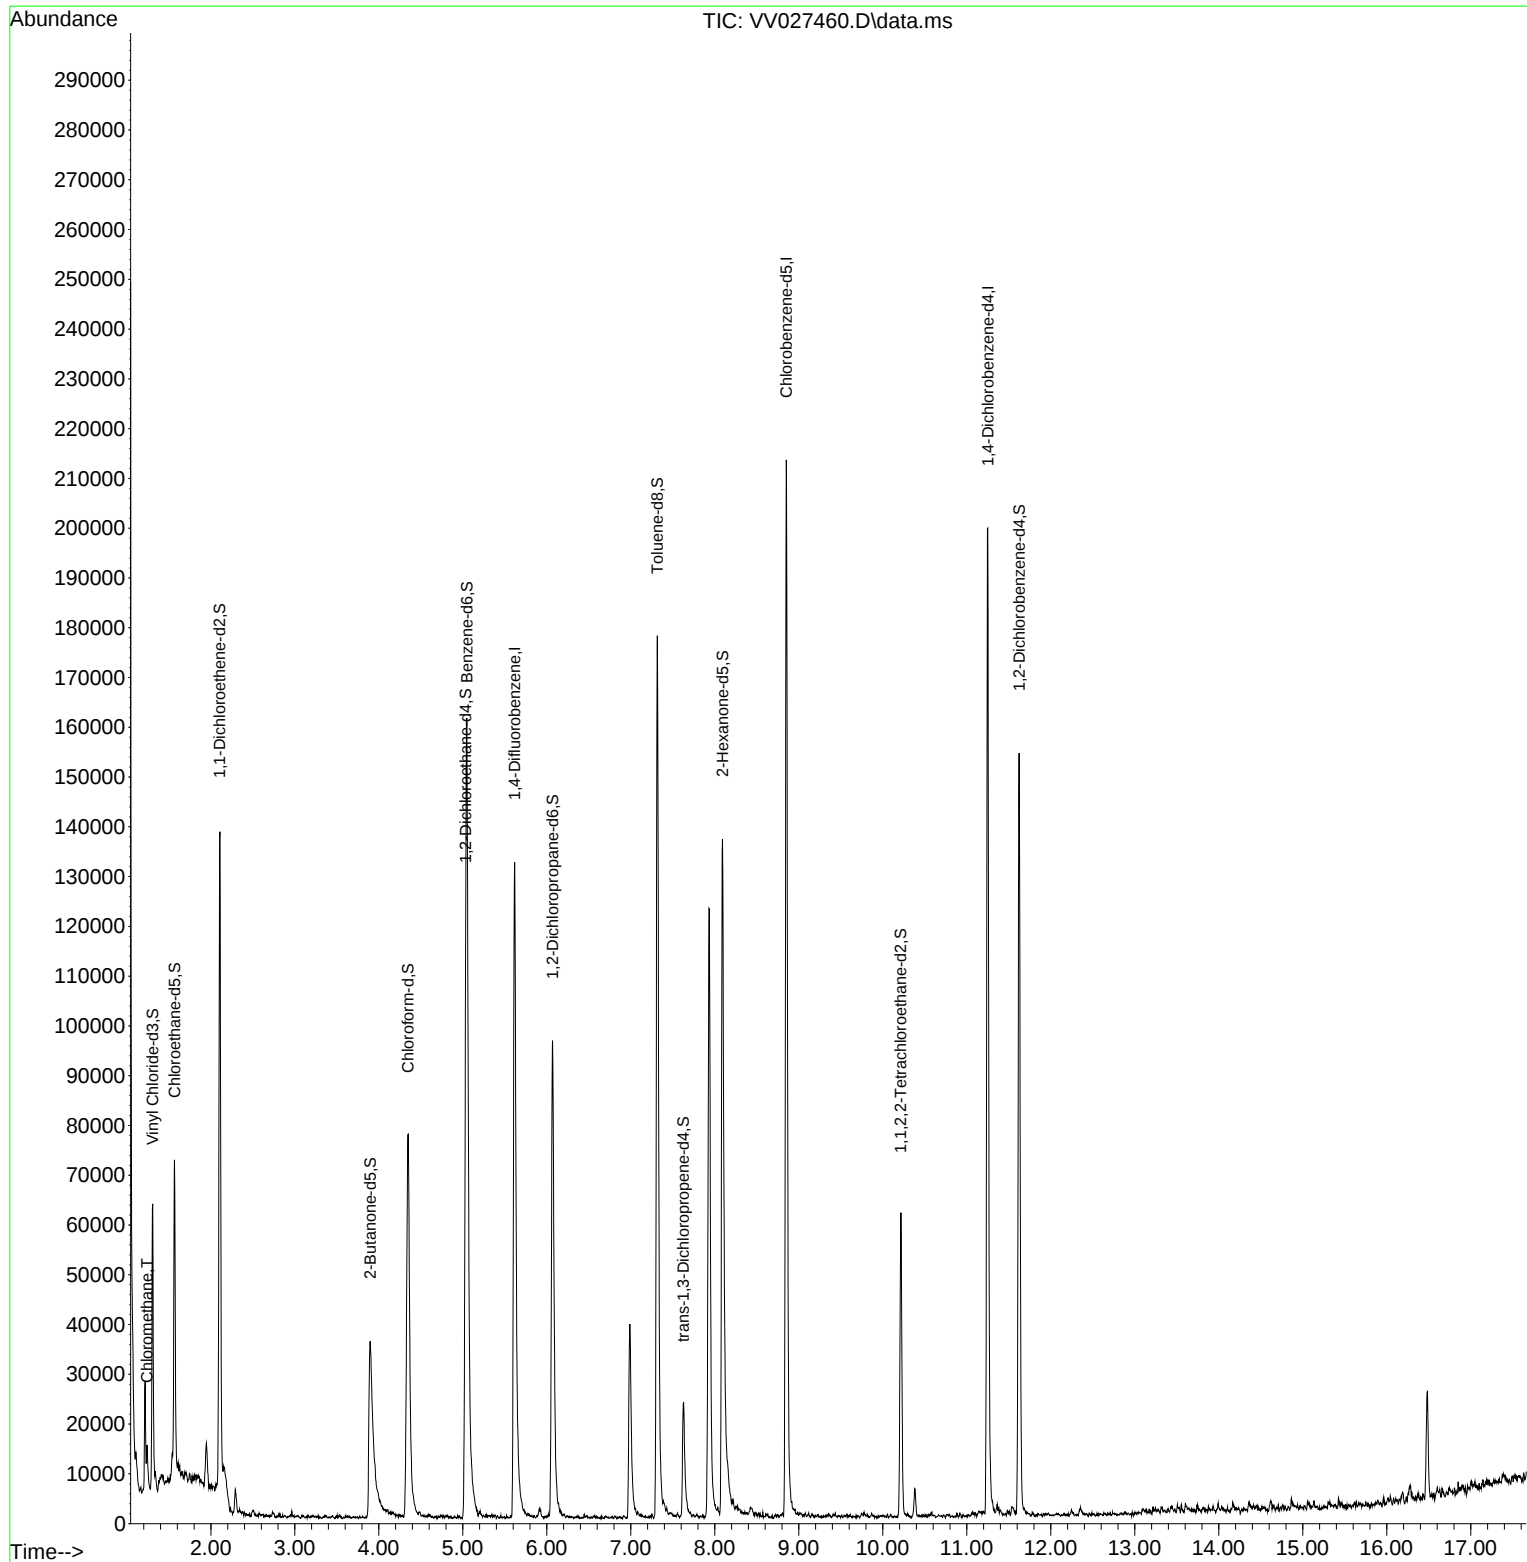

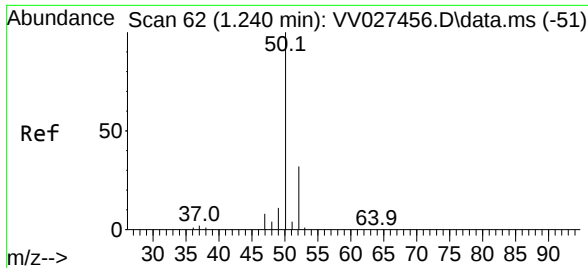

#3
 Chloromethane
 Concen: 0.642 ug/L
 RT: 1.240 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: VV027460.D
 Acq: 22 Aug 2022 12:04

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9C2

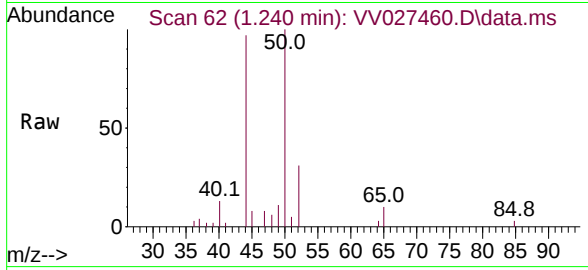

Tgt Ion:	50	Resp:	6966
Ion Ratio	Lower	Upper	
50	100		
52	31.5	22.8	42.4

