

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027470.D
 Acq On : 22 Aug 2022 16:10
 Operator : SY/MD
 Sample : N4252-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D1

Quant Time: Aug 23 03:13:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Aug 23 03:03:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	118437	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	117915	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52055	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	37438	4.441	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.800%
7) Chloroethane-d5	1.564	69	39069	6.333	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	126.600%
11) 1,1-Dichloroethene-d2	2.105	63	70806	3.602	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.000%
20) 2-Butanone-d5	3.905	46	33474	31.910	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	63.820%
24) Chloroform-d	4.346	84	78596	4.663	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	5.031	65	37370	5.125	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.047	84	147462	4.515	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%
36) 1,2-Dichloropropane-d6	6.069	67	44669	4.704	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.000%
41) Toluene-d8	7.317	98	117732	3.992	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.800%
43) trans-1,3-Dichloroprop...	7.625	79	13739	4.226	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.091	63	44830	41.888	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.780%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	29737	4.918	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	39343	5.098	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds						Qvalue
3) Chloromethane	1.240	50	3913	0.357	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027470.D
Acq On : 22 Aug 2022 16:10
Operator : SY/MD
Sample : N4252-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D1

Quant Time: Aug 23 03:13:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Aug 23 03:03:07 2022
Response via : Initial Calibration

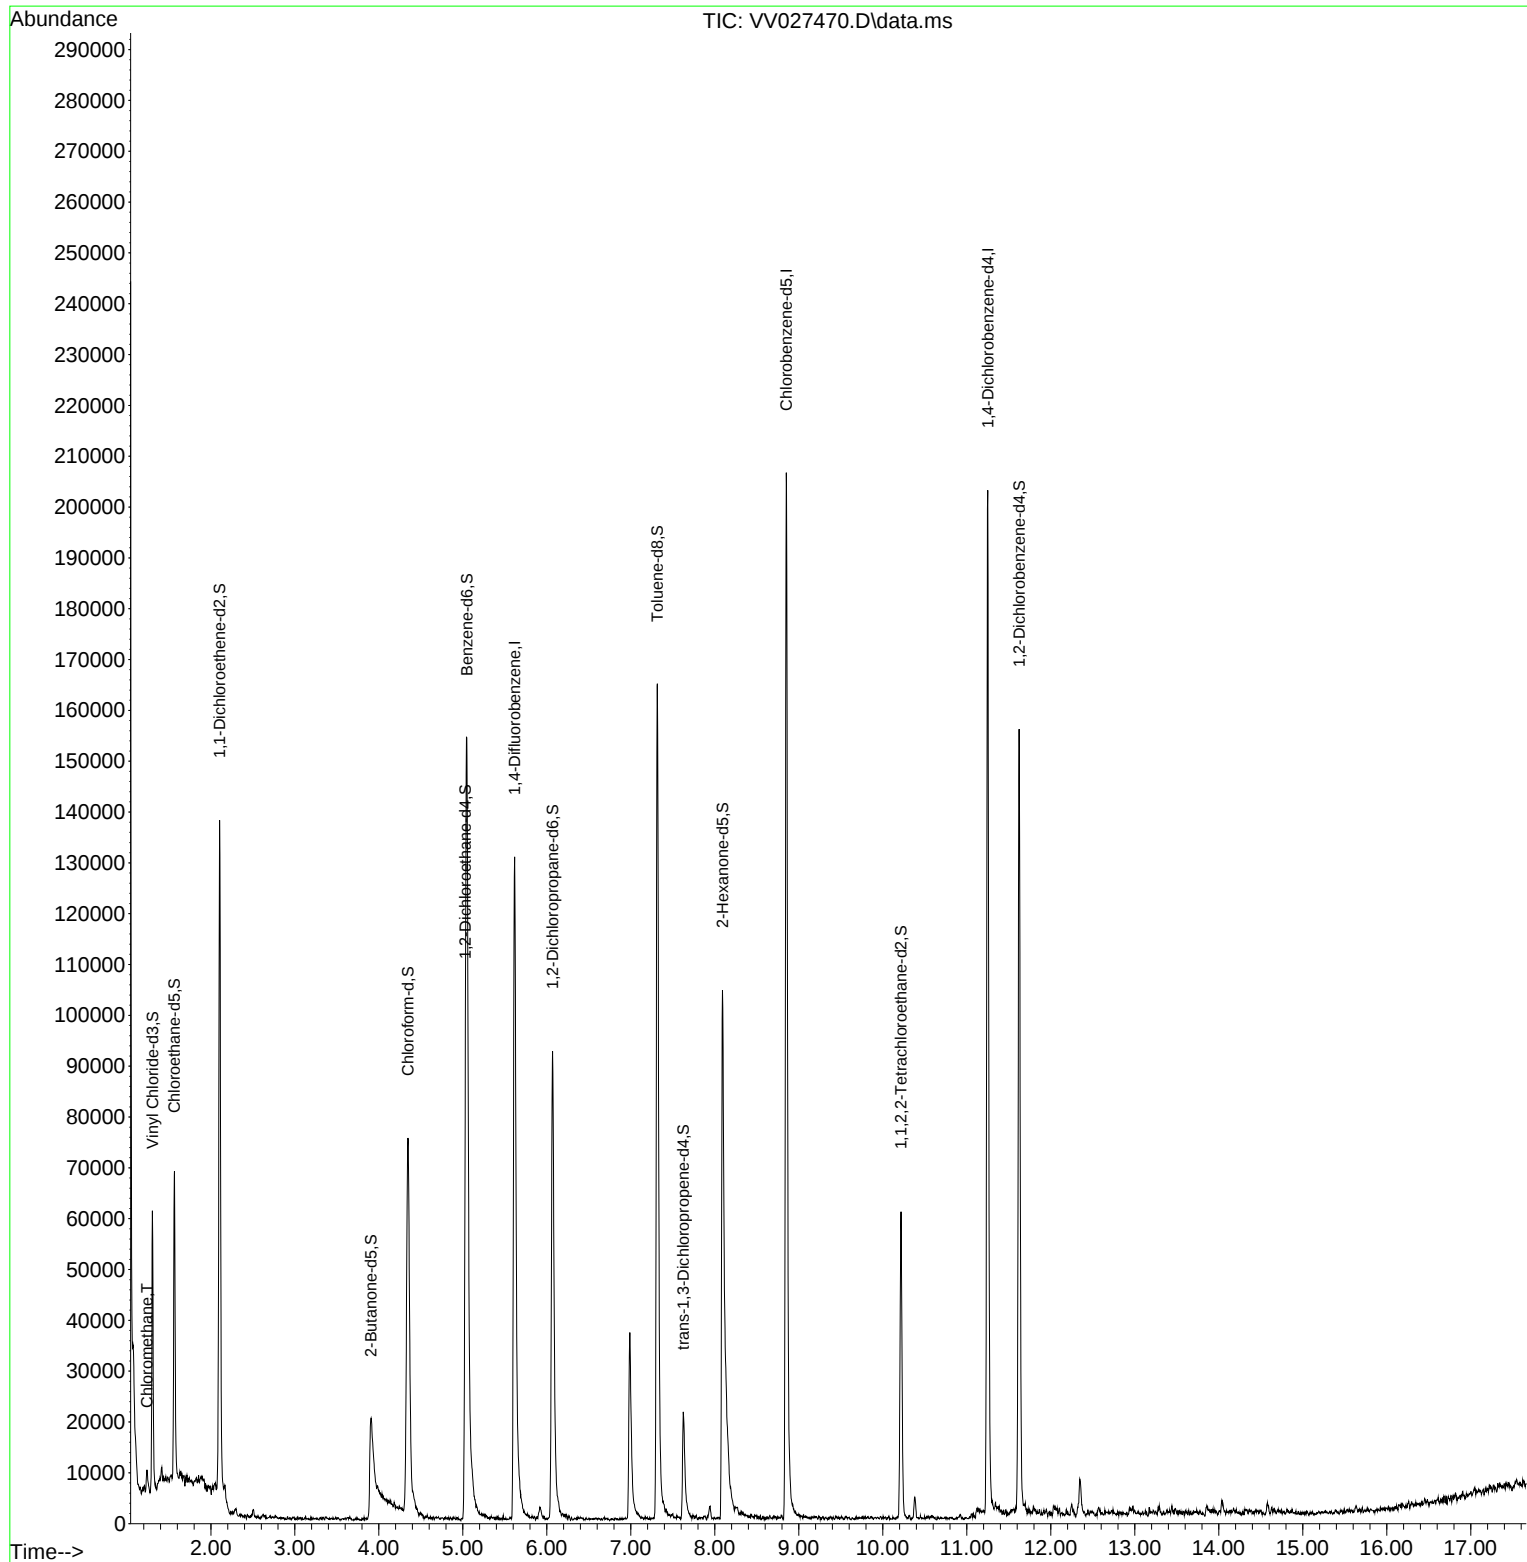

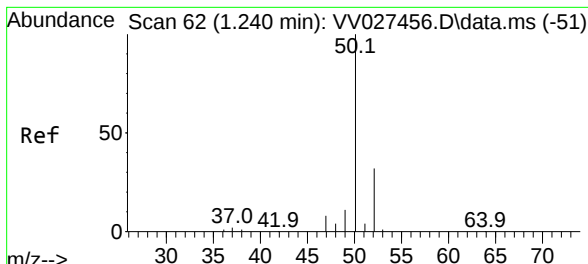

#3
 Chloromethane
 Concen: 0.357 ug/L
 RT: 1.240 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: VV027470.D
 Acq: 22 Aug 2022 16:10

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D1

Tgt Ion: 50 Resp: 3913
 Ion Ratio Lower Upper
 50 100
 52 34.3 22.8 42.4

