

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027465.D
 Acq On : 22 Aug 2022 14:07
 Operator : SY/MD
 Sample : N4252-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9C7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	48	54	72	rBV	114117	116537	1.43%	0.882%
2	1.307	75	83	122	rBV	1063791	1256594	15.37%	9.512%
3	2.105	322	331	344	rBV2	143568	223728	2.74%	1.693%
4	2.757	522	534	549	rBV	196807	343721	4.20%	2.602%
5	3.902	873	890	908	rBV	3481708	8174768	100.00%	61.877%
6	4.342	1013	1027	1062	rBV2	74747	193895	2.37%	1.468%
7	5.043	1230	1245	1286	rBV2	157159	416150	5.09%	3.150%
8	5.616	1412	1423	1457	rBV	126918	278208	3.40%	2.106%
9	5.911	1503	1515	1546	rBV	228016	473891	5.80%	3.587%
10	6.069	1552	1564	1593	rBV2	90003	197847	2.42%	1.498%
11	7.317	1939	1952	1974	rBV	165302	310806	3.80%	2.353%
12	8.091	2183	2193	2226	rBV	125903	269047	3.29%	2.036%
13	8.853	2418	2430	2452	rBV	195920	335935	4.11%	2.543%
14	10.217	2843	2854	2866	rBV	60659	93729	1.15%	0.709%
15	11.249	3164	3175	3196	rBV	185361	296670	3.63%	2.246%
16	11.622	3280	3291	3307	rBV	143111	229758	2.81%	1.739%




Sum of corrected areas: 13211284

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027465.D
Acq On : 22 Aug 2022 14:07
Operator : SY/MD
Sample : N4252-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

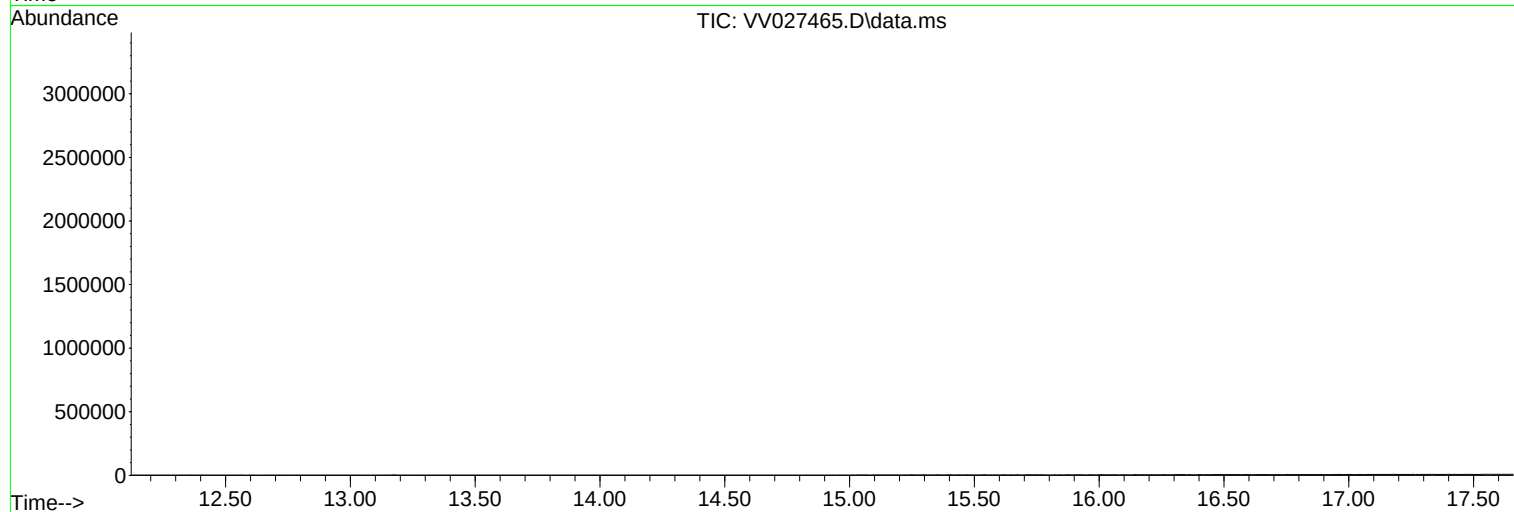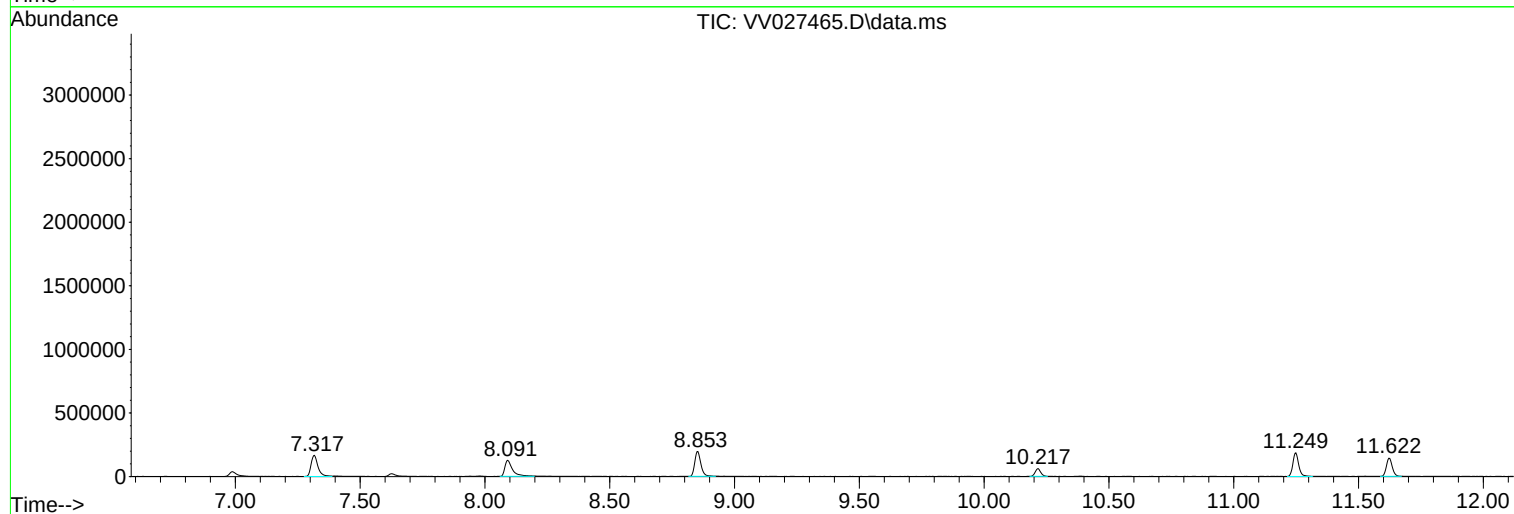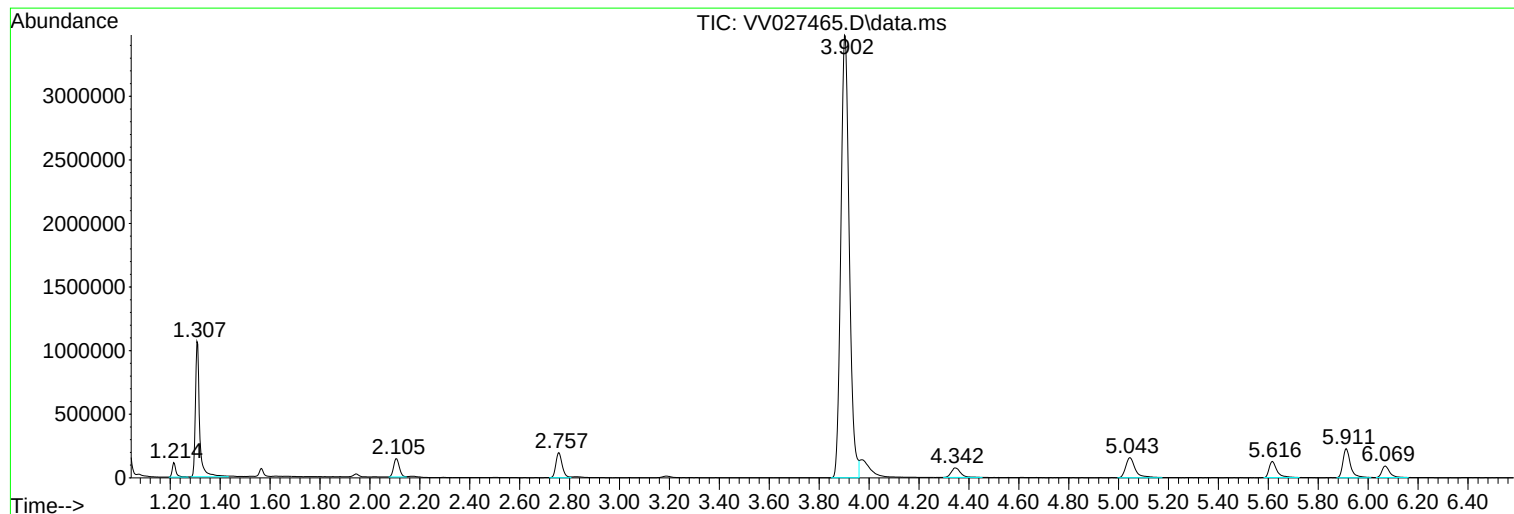

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027465.D
Acq On : 22 Aug 2022 14:07
Operator : SY/MD
Sample : N4252-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1-chloro-1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.214	2.09 ug/L	116537	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	83
2			Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	74
3			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	40
4			2,2-Difluoropropionic acid	110	C3H4F2O2	000373-96-6	4
5			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	4

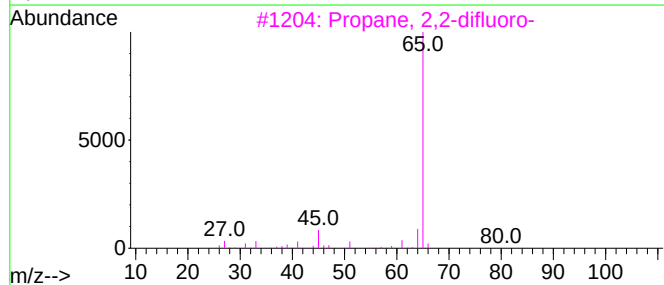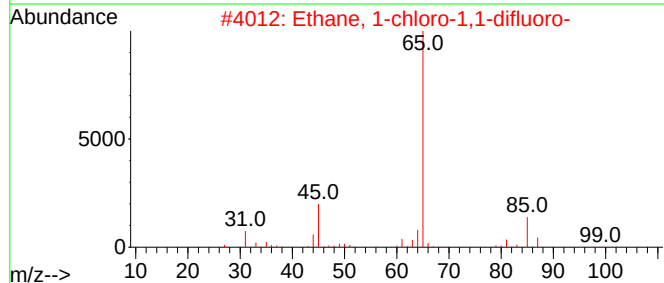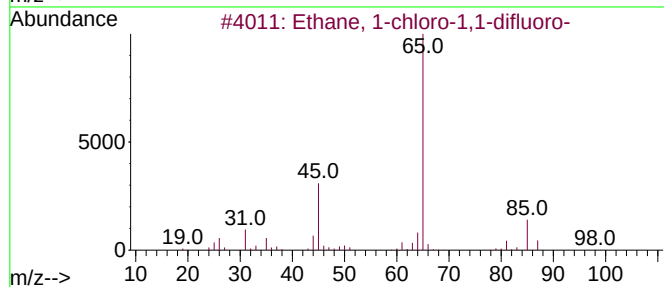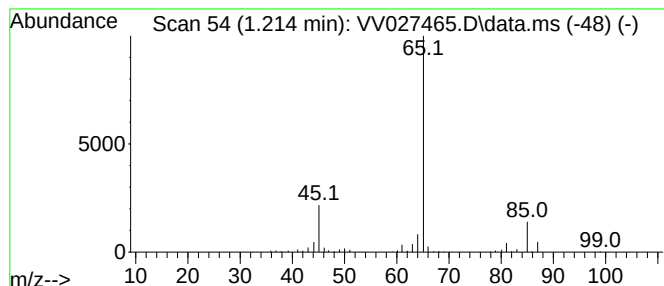

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027465.D
Acq On : 22 Aug 2022 14:07
Operator : SY/MD
Sample : N4252-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1-chlor...	1.214	2.1	ug/L	116537	1	5.616	278208	5.0