

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027468.D
 Acq On : 22 Aug 2022 15:21
 Operator : SY/MD
 Sample : N4252-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9C9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	75	rVB2	5871	7931	1.26%	0.177%
2	1.304	75	82	98	rVB	54337	64144	10.21%	1.433%
3	1.568	153	164	179	rVB	61739	75337	11.99%	1.683%
4	1.947	274	282	294	rVB	21029	31894	5.08%	0.713%
5	2.108	317	332	345	rBV	146524	237598	37.83%	5.309%
6	2.172	345	352	363	rVB	6945	15145	2.41%	0.338%
7	2.761	525	535	548	rBV2	12410	22558	3.59%	0.504%
8	3.909	876	892	912	rBV2	236736	628108	100.00%	14.034%
9	4.346	1011	1028	1048	rBV2	76398	193905	30.87%	4.332%
10	5.047	1231	1246	1273	rBV3	152826	404419	64.39%	9.036%
11	5.616	1412	1423	1451	rBV2	121621	267526	42.59%	5.977%
12	5.912	1502	1515	1548	rBV	284143	603417	96.07%	13.482%
13	6.069	1550	1564	1591	rVB	91243	199634	31.78%	4.460%
14	6.989	1839	1850	1872	rBV2	37158	77943	12.41%	1.742%
15	7.317	1940	1952	1971	rBV	166712	310722	49.47%	6.943%
16	7.625	2036	2048	2070	rBV	22951	45825	7.30%	1.024%
17	7.976	2148	2157	2175	rVB	22378	42240	6.72%	0.944%
18	8.092	2182	2193	2223	rBV	112515	273005	43.46%	6.100%
19	8.854	2417	2430	2447	rBV	193313	333015	53.02%	7.441%
20	10.217	2840	2854	2868	rBV2	57977	95899	15.27%	2.143%
21	11.249	3162	3175	3191	rBV	187346	300932	47.91%	6.724%
22	11.622	3279	3291	3308	rBV	148636	244413	38.91%	5.461%




Sum of corrected areas: 4475610

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027468.D
Acq On : 22 Aug 2022 15:21
Operator : SY/MD
Sample : N4252-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

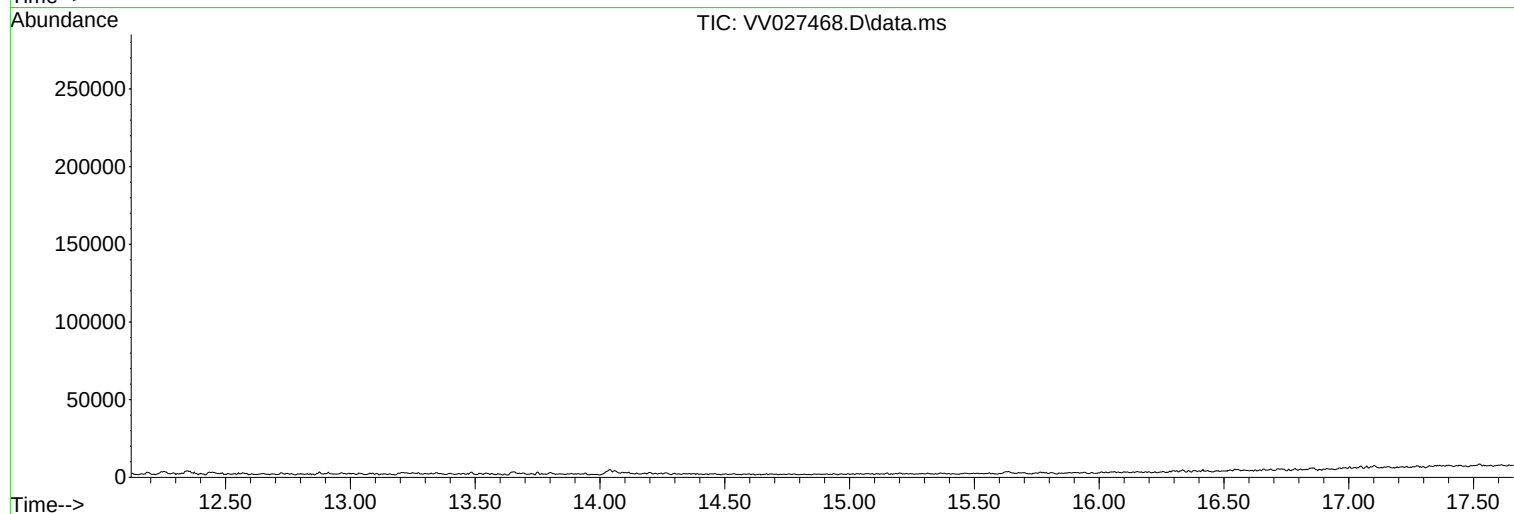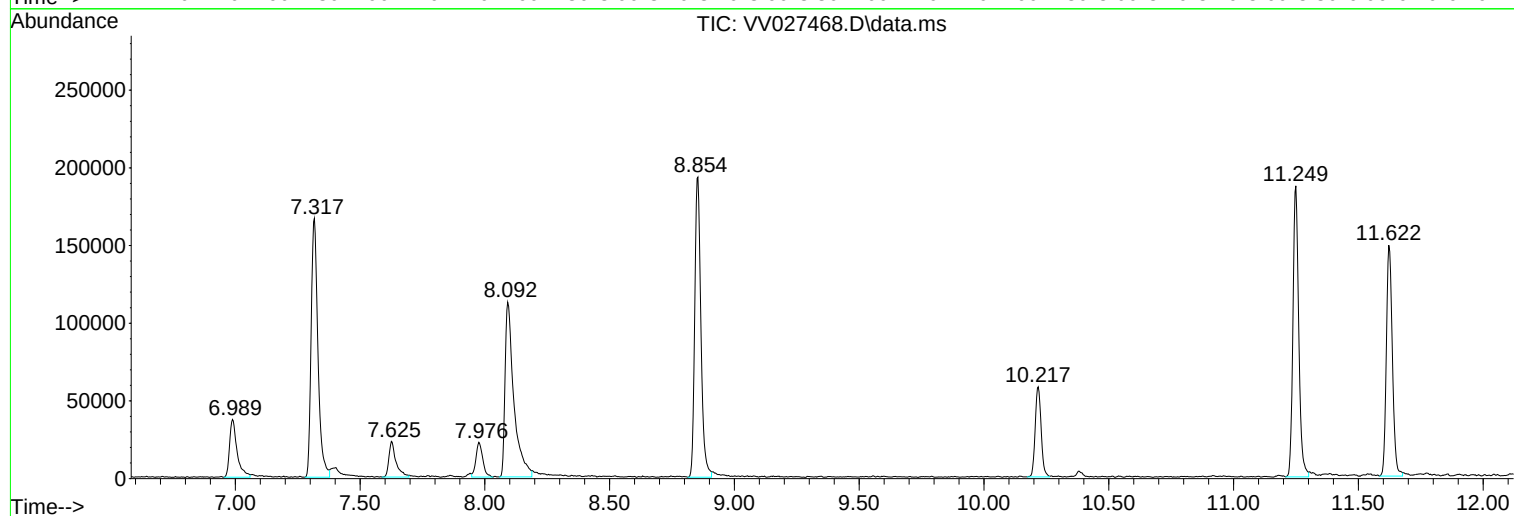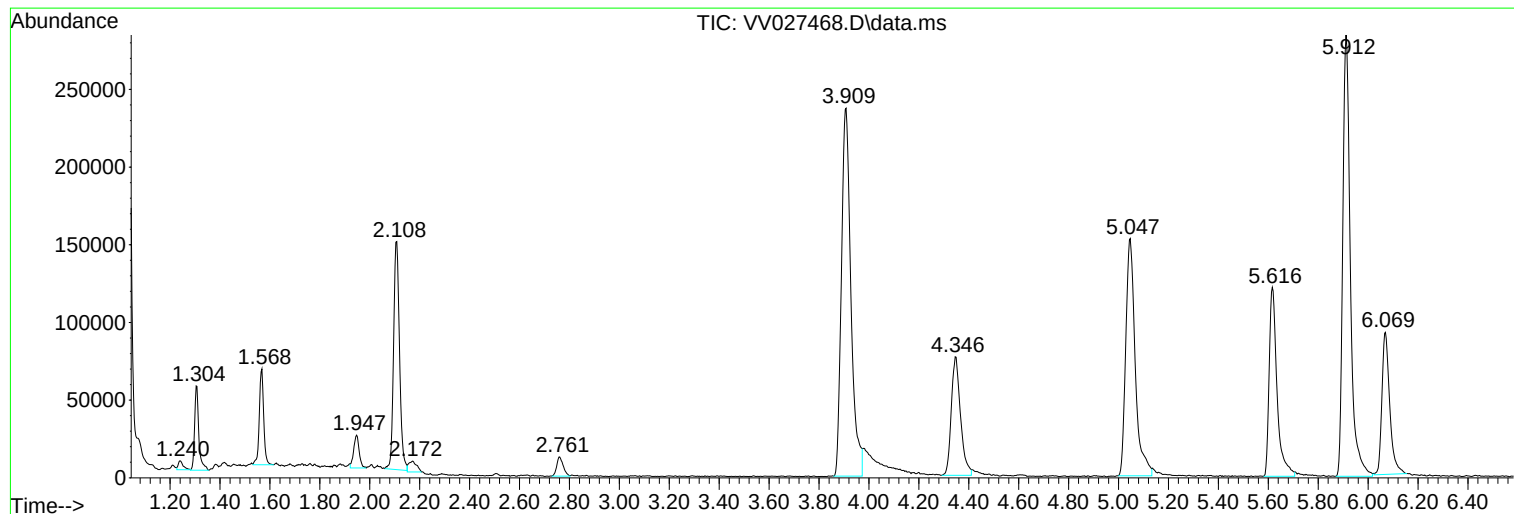

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027468.D
Acq On : 22 Aug 2022 15:21
Operator : SY/MD
Sample : N4252-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.947	0.60 ug/L	31894	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	91
2			1,4-Pentadiene, 3-methyl-	82	C6H10	001115-08-8	22
3			cis-4-Hydroxycyclohexanecarboxyl...	126	C7H10O2	004350-84-9	12
4			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	10
5			5-Ethoxy-3-methyl-1,3-pentadiene	126	C8H14O	1000432-35-5	10

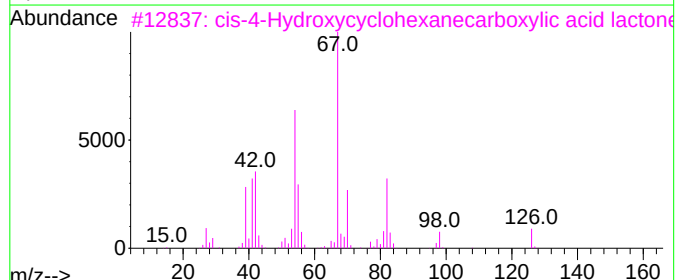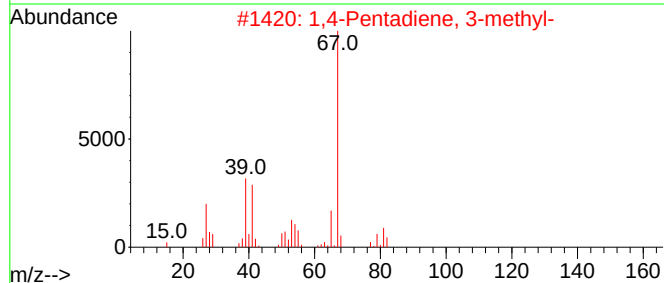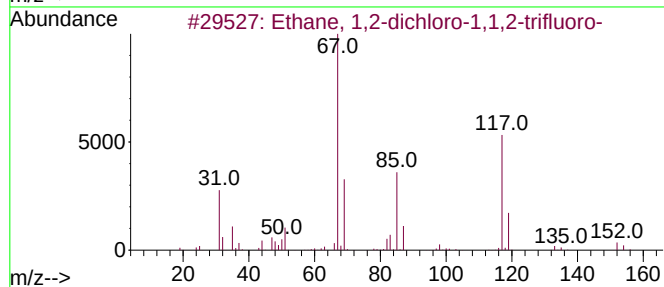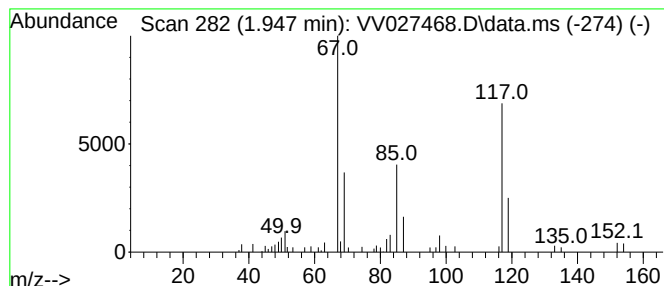

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027468.D
Acq On : 22 Aug 2022 15:21
Operator : SY/MD
Sample : N4252-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9C9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,2-dic...	1.947	0.6	ug/L	31894	1	5.616	267526	5.0