

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027470.D
 Acq On : 22 Aug 2022 16:10
 Operator : SY/MD
 Sample : N4252-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EX9D1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	73	rVB2	4573	6511	1.58%	0.201%
2	1.304	74	82	93	rBV	55352	59463	14.45%	1.835%
3	1.568	156	164	174	rBV	60208	71616	17.40%	2.210%
4	2.105	320	331	347	rBV	131533	189784	46.12%	5.856%
5	3.908	879	892	912	rBV3	19902	69460	16.88%	2.143%
6	4.346	1012	1028	1057	rBV2	73335	190890	46.39%	5.890%
7	5.043	1230	1245	1280	rBV3	153794	411484	100.00%	12.696%
8	5.616	1412	1423	1458	rBV	130229	288378	70.08%	8.898%
9	5.915	1509	1516	1526	rBV	2154	4249	1.03%	0.131%
10	6.069	1551	1564	1591	rBV2	91738	201004	48.85%	6.202%
11	6.989	1840	1850	1874	rBV2	36497	74824	18.18%	2.309%
12	7.317	1939	1952	1981	rBV	164258	313841	76.27%	9.683%
13	7.625	2039	2048	2071	rBV2	21040	43388	10.54%	1.339%
14	8.091	2184	2193	2238	rBV	103937	272354	66.19%	8.403%
15	8.850	2419	2429	2452	rBV	205799	361213	87.78%	11.145%
16	10.217	2841	2854	2868	rBV	60281	98214	23.87%	3.030%
17	10.381	2896	2905	2912	rBV4	4183	6081	1.48%	0.188%
18	11.249	3164	3175	3191	rBV	201170	319174	77.57%	9.848%
19	11.622	3280	3291	3307	rBV	153446	247803	60.22%	7.646%
20	12.345	3511	3516	3530	rVB10	6697	11270	2.74%	0.348%




Sum of corrected areas: 3241001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027470.D
Acq On : 22 Aug 2022 16:10
Operator : SY/MD
Sample : N4252-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

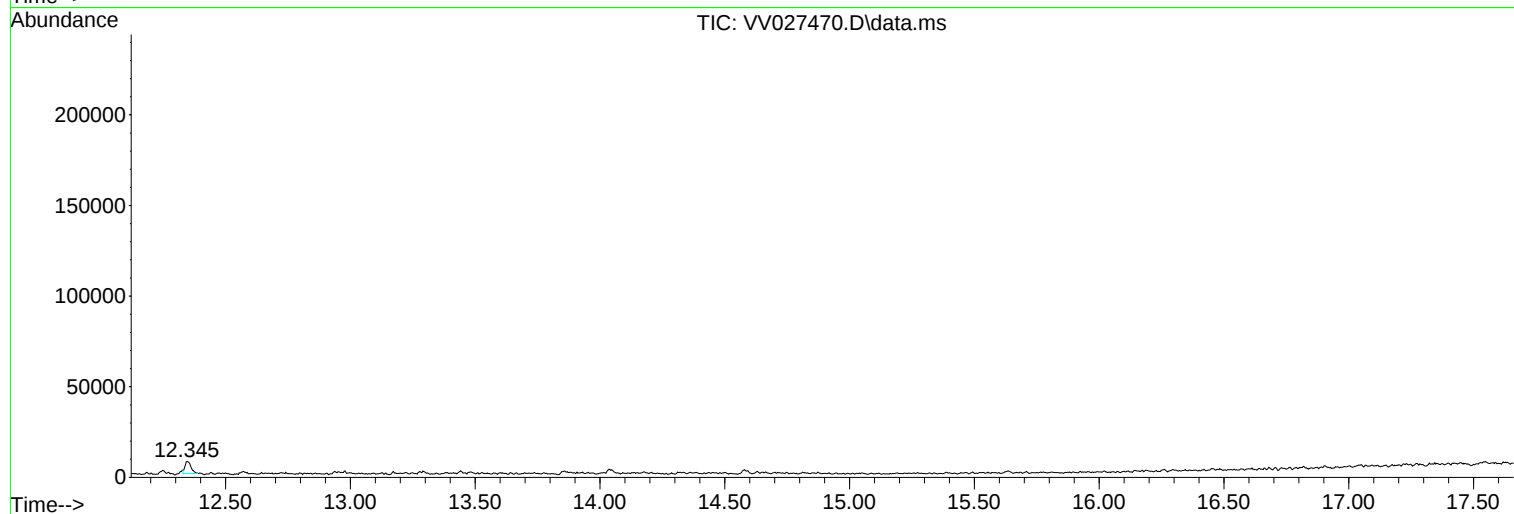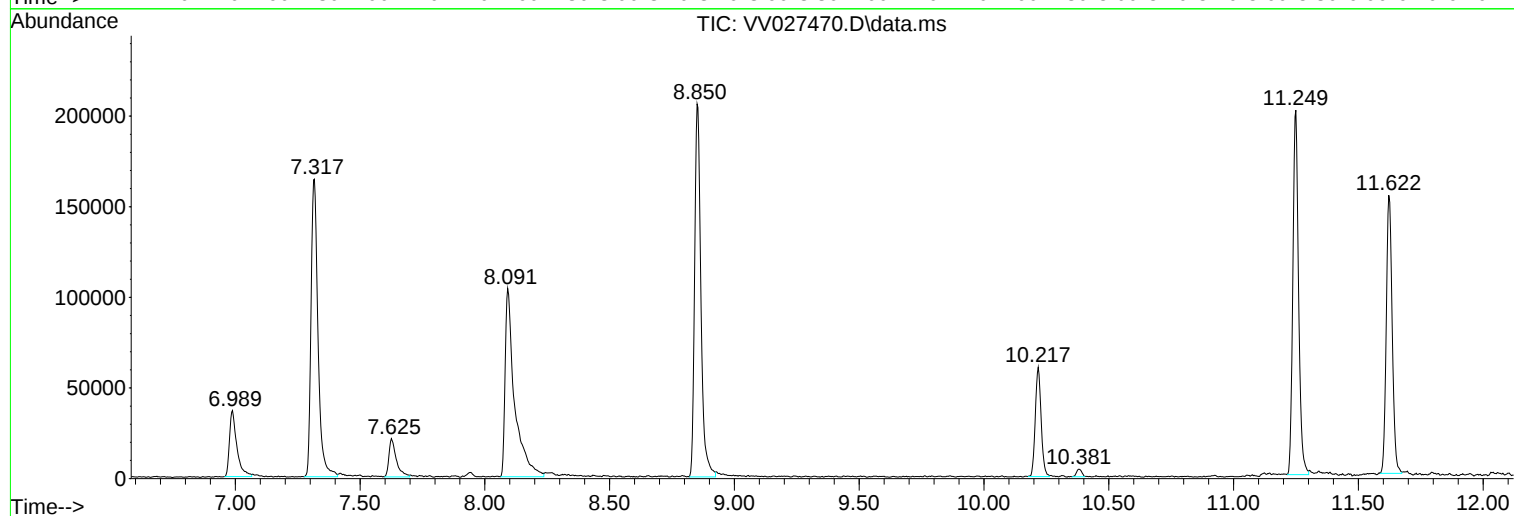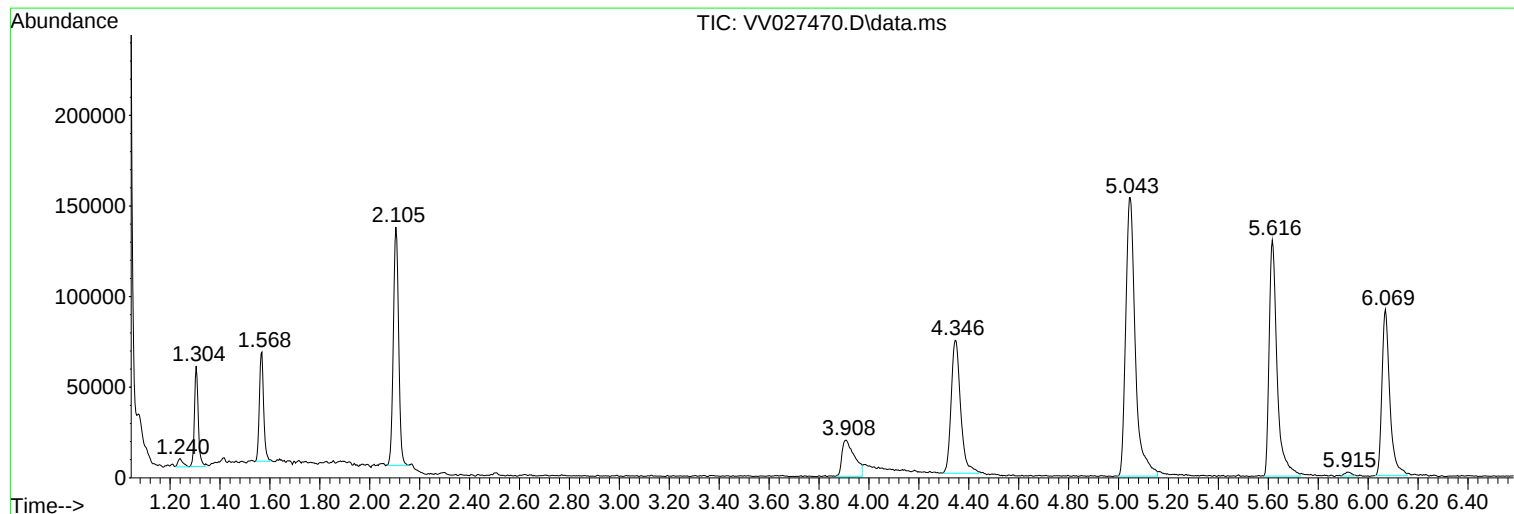

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027470.D
Acq On : 22 Aug 2022 16:10
Operator : SY/MD
Sample : N4252-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027470.D
Acq On : 22 Aug 2022 16:10
Operator : SY/MD
Sample : N4252-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EX9D1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------