

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027475.D
 Acq On : 22 Aug 2022 18:13
 Operator : SY/MD
 Sample : N4253-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	54071	62162	15.48%	1.935%
2	1.568	157	164	176	rVB	60545	68405	17.04%	2.129%
3	2.105	321	331	345	rVB	126187	184552	45.97%	5.745%
4	3.908	877	892	918	rBV3	45220	158275	39.43%	4.927%
5	4.346	1013	1028	1049	rBV	72822	191931	47.81%	5.974%
6	5.047	1228	1246	1278	rBV2	152390	401445	100.00%	12.496%
7	5.616	1412	1423	1450	rBV	119192	261028	65.02%	8.125%
8	5.915	1507	1516	1545	rVB5	19691	48526	12.09%	1.510%
9	6.069	1551	1564	1591	rBV2	91524	198681	49.49%	6.184%
10	6.989	1837	1850	1874	rBV2	34698	72993	18.18%	2.272%
11	7.317	1941	1952	1975	rBV	158817	300785	74.93%	9.363%
12	7.628	2037	2049	2067	rBV2	21576	43008	10.71%	1.339%
13	8.091	2182	2193	2234	rBV	124094	276018	68.76%	8.592%
14	8.850	2419	2429	2451	rBV	193926	331052	82.47%	10.305%
15	10.217	2843	2854	2869	rBV	57854	94618	23.57%	2.945%
16	11.249	3163	3175	3192	rBV	176181	278204	69.30%	8.660%
17	11.625	3277	3292	3314	rBV	141045	230250	57.36%	7.167%
18	12.349	3511	3517	3526	rBV10	2754	4056	1.01%	0.126%
19	15.680	4546	4553	4559	rVB6	5114	6636	1.65%	0.207%




Sum of corrected areas: 3212625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027475.D
Acq On : 22 Aug 2022 18:13
Operator : SY/MD
Sample : N4253-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

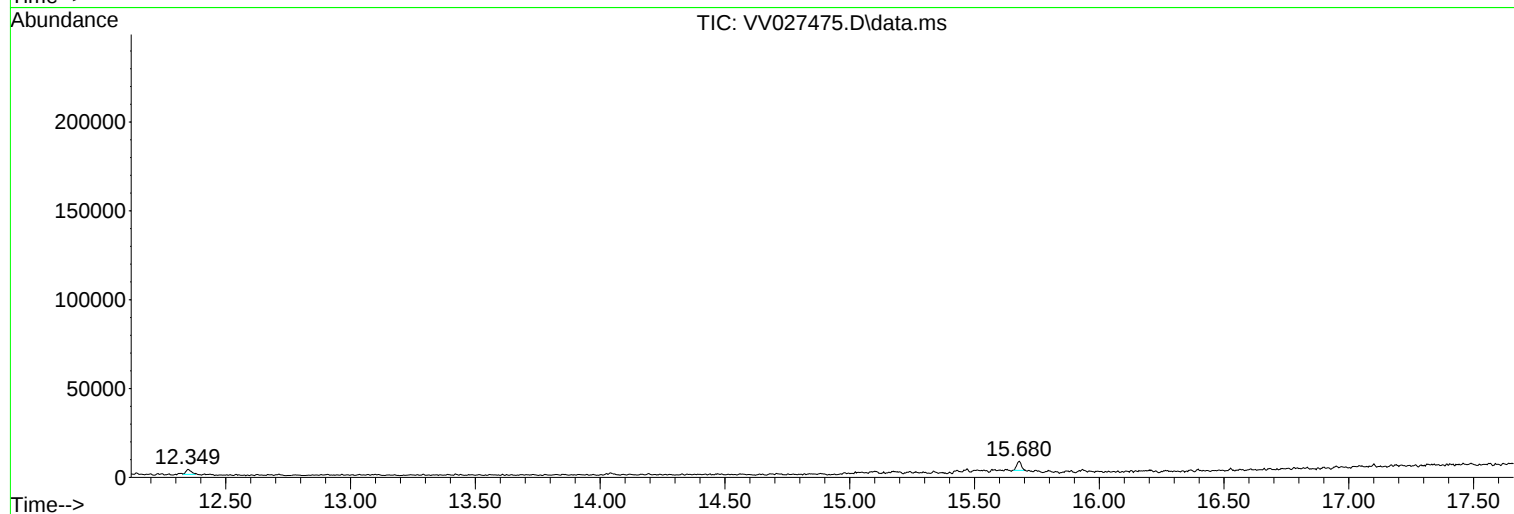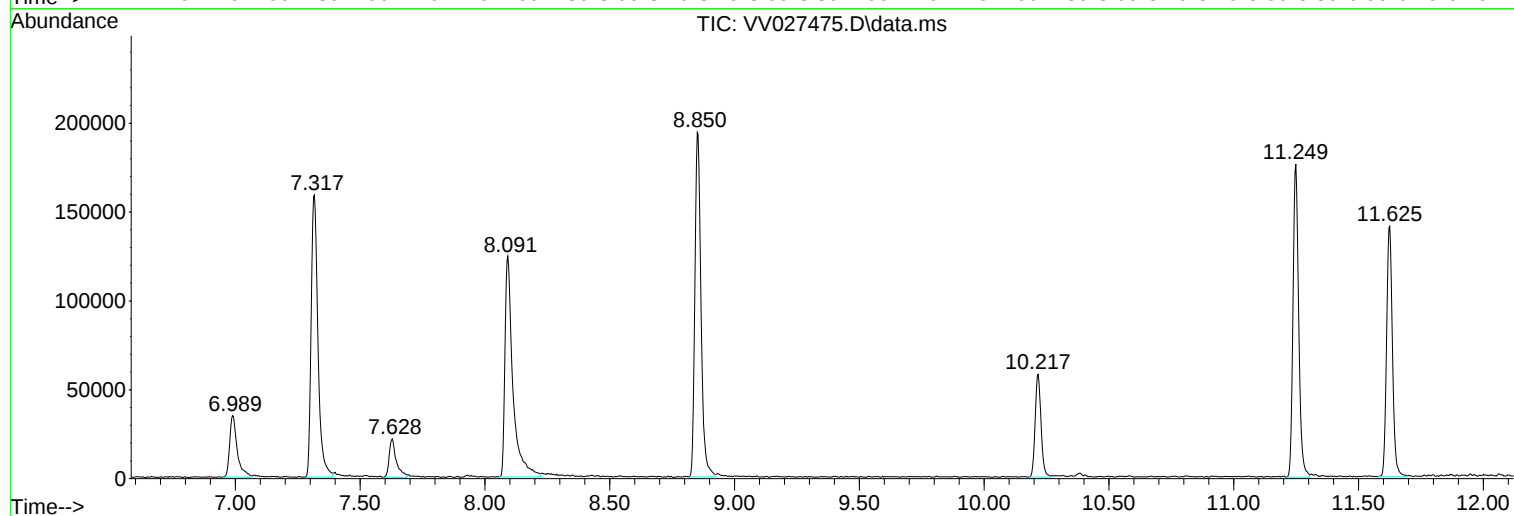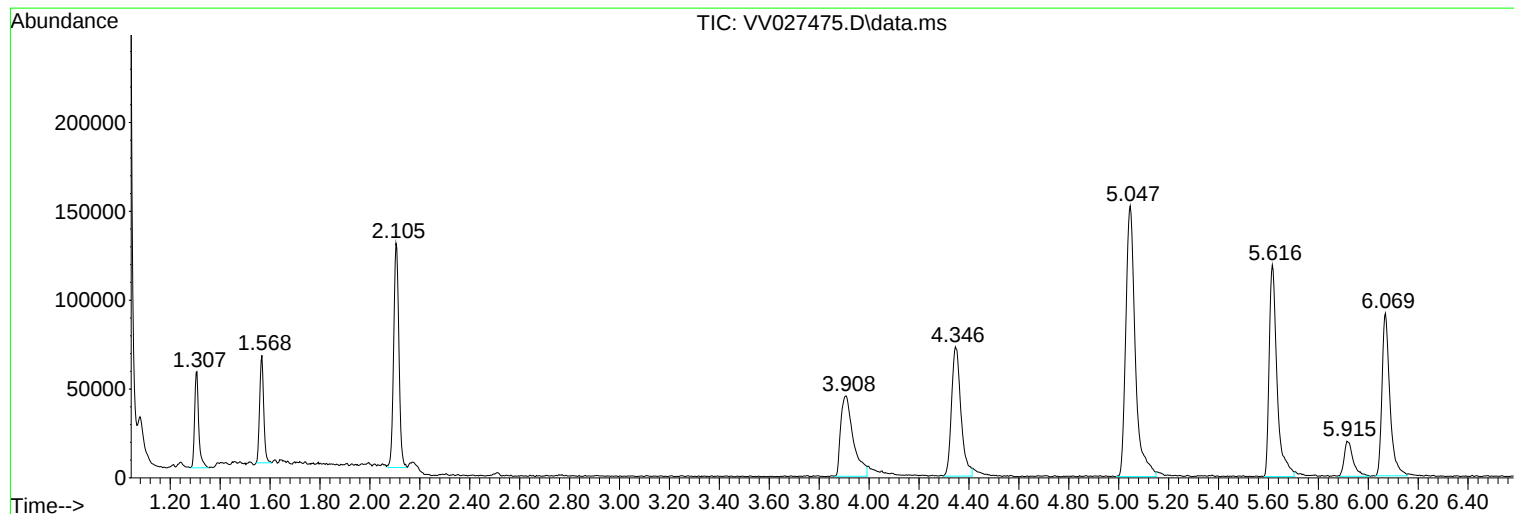

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027475.D
Acq On : 22 Aug 2022 18:13
Operator : SY/MD
Sample : N4253-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
Data File : VV027475.D
Acq On : 22 Aug 2022 18:13
Operator : SY/MD
Sample : N4253-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
