


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082222\
 Data File : VV027455.D
 Acq On : 22 Aug 2022 09:16
 Operator : SY/MD
 Sample : BFB357
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB357

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 27 03:12:26 2022

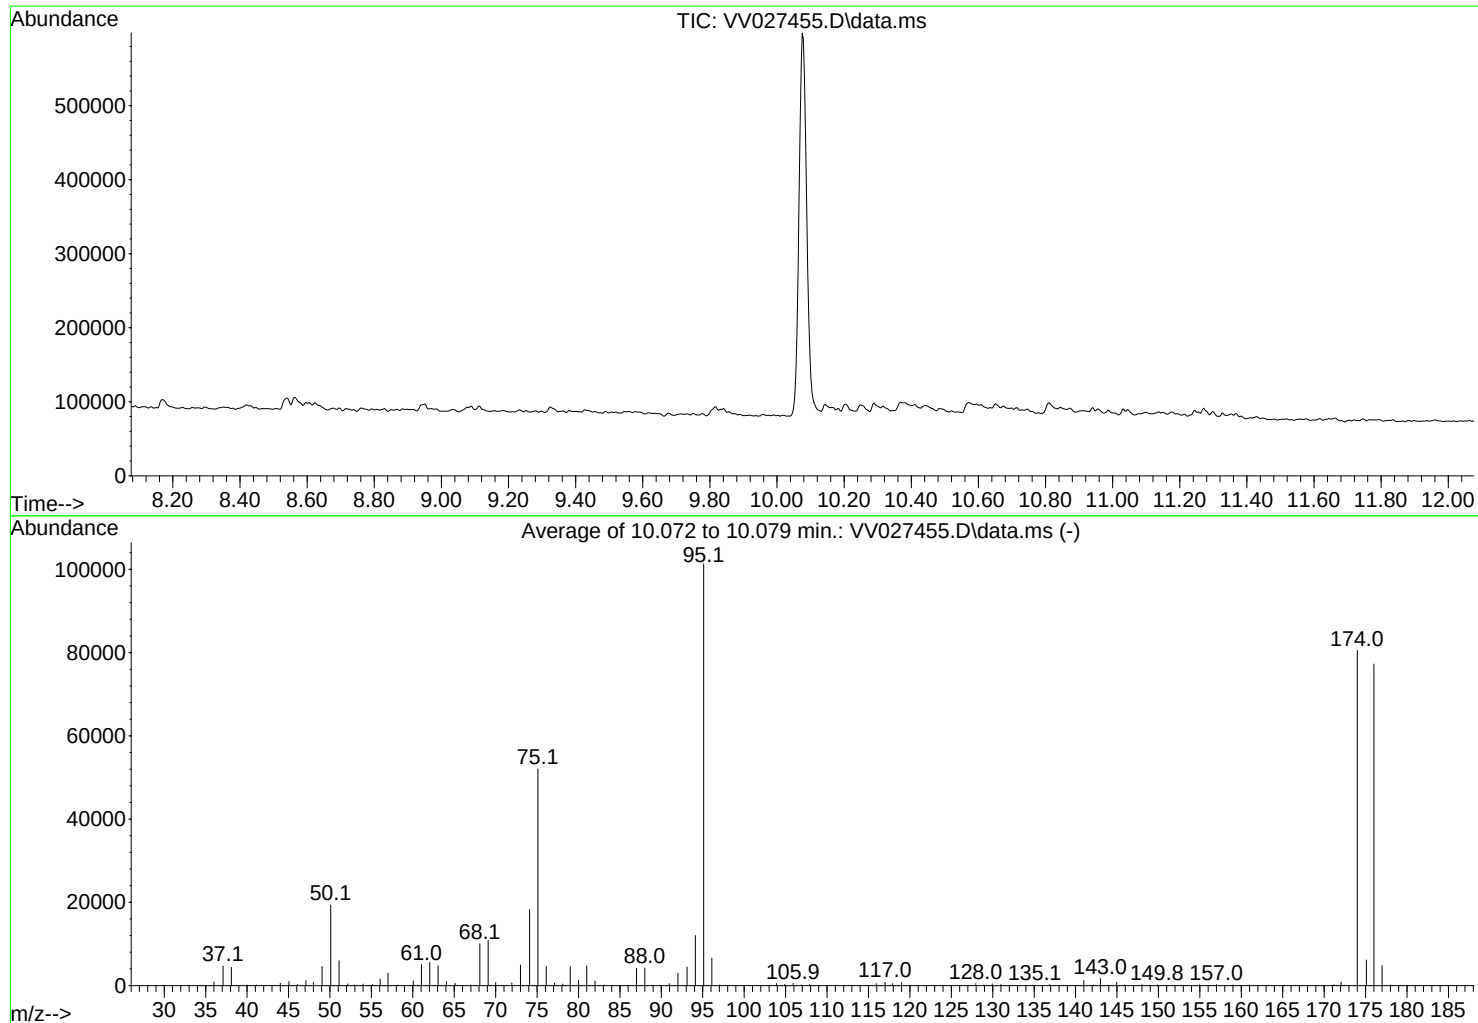

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	19315	PASS
75	95	30	80	51.3	52019	PASS
95	95	100	100	100.0	101347	PASS
96	95	5	9	6.5	6601	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.4	80480	PASS
175	174	5	9	7.6	6116	PASS
176	174	95	105	96.0	77272	PASS
177	176	5	10	6.2	4818	PASS

m/z	Abundance
36.00	305.0
37.90	130.0
40.00	79520.0
42.80	103.0
44.00	716.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

m/z	Abundance
36.00	1082.0
37.10	4607.0
38.10	4298.0
40.00	78824.0
41.10	129.0
42.00	128.0
43.00	135.0
44.00	1266.0
45.00	897.0
46.10	282.0
47.10	1276.0
48.00	713.0
49.00	4302.0
50.10	18112.0
51.10	5955.0
52.10	395.0
52.90	179.0
54.00	341.0
54.80	225.0
55.20	211.0
56.10	1526.0
57.00	2947.0
58.20	118.0
60.00	987.0
61.10	4862.0
62.00	5569.0
63.00	4602.0
64.10	959.0
65.10	502.0
66.10	111.0
67.00	263.0
68.10	9666.0
69.10	10433.0
70.00	735.0
72.00	552.0
73.00	4721.0
74.10	17168.0
75.10	49192.0
76.10	4565.0
77.10	587.0
78.10	571.0
79.00	4246.0
80.00	1153.0
81.00	4389.0
82.00	1008.0
83.10	128.0
86.00	179.0
87.00	3765.0
88.00	4158.0
90.90	421.0
92.00	3174.0
93.10	4303.0
94.10	11686.0
95.10	97160.0
96.10	6483.0
97.10	163.0
103.90	446.0
104.90	203.0
105.90	505.0
106.90	157.0
107.90	265.0
110.10	109.0
111.20	140.0
115.90	406.0
117.00	754.0
117.90	420.0
119.00	706.0
127.90	425.0
128.90	179.0
129.90	406.0
131.00	218.0
134.80	186.0
136.90	259.0
141.00	1212.0
143.00	1604.0
143.80	156.0
144.90	772.0
145.90	189.0
148.00	195.0
149.00	140.0
149.80	177.0
152.70	113.0
155.00	205.0
157.00	246.0
159.00	135.0
161.00	175.0
171.20	280.0
172.10	689.0
174.00	75312.0
175.10	5890.0
176.00	71856.0
177.00	4677.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

178.10

133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

m/z	Abundance
36.10	1176.0
37.10	4843.0
38.10	4467.0
40.00	79696.0
41.20	141.0
44.00	1288.0
45.10	1028.0
46.10	304.0
47.10	1235.0
48.00	796.0
49.10	4800.0
50.10	19968.0
51.10	6198.0
52.10	398.0
53.00	152.0
54.00	338.0
55.10	256.0
56.00	1586.0
57.00	3100.0
58.20	136.0
60.10	1133.0
61.10	5258.0
62.00	5801.0
63.00	4968.0
64.10	955.0
65.10	545.0
67.00	281.0
68.10	10328.0
69.10	11212.0
70.00	728.0
71.90	643.0
73.00	5052.0
74.10	18840.0
75.10	53944.0
76.10	4786.0
77.10	602.0
78.10	553.0
79.00	4726.0
80.00	1330.0
81.00	4871.0
82.00	1131.0
83.10	172.0
85.90	141.0
87.00	4263.0
88.00	4393.0
90.90	458.0
92.00	3081.0
93.10	4653.0
94.10	12373.0
95.10	104520.0
96.10	6866.0
97.00	149.0
103.90	485.0
104.90	249.0
105.90	533.0
106.90	187.0
107.90	280.0
110.10	115.0
111.10	132.0
115.90	477.0
117.00	806.0
117.90	467.0
119.00	728.0
128.00	491.0
128.90	176.0
130.00	447.0
131.00	261.0
135.10	169.0
136.90	228.0
141.00	1251.0
142.20	203.0
143.00	1750.0
143.90	138.0
144.90	875.0
145.90	163.0
148.00	237.0
148.90	115.0
149.90	168.0
152.60	118.0
153.10	107.0
154.90	231.0
157.00	235.0
158.90	151.0
161.00	188.0
171.20	306.0
172.10	836.0
174.00	83136.0
175.10	6274.0
176.00	79744.0
177.00	4965.0
178.00	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357

m/z	Abundance
36.10	1201.0
37.10	4720.0
38.10	4410.0
40.00	80424.0
41.20	111.0
44.00	1225.0
45.10	1023.0
46.10	246.0
47.10	1105.0
48.00	771.0
49.10	4661.0
50.10	19864.0
51.10	5815.0
52.20	400.0
53.00	141.0
54.00	385.0
55.10	274.0
56.00	1560.0
57.00	2898.0
58.20	176.0
60.10	1222.0
61.00	5102.0
62.10	5378.0
63.10	4728.0
64.00	885.0
65.10	596.0
68.10	10197.0
69.10	10916.0
70.00	705.0
71.90	657.0
73.00	4887.0
74.10	18704.0
75.10	52920.0
76.10	4416.0
77.10	646.0
79.00	4661.0
80.00	1386.0
81.00	5028.0
82.00	1115.0
83.10	184.0
87.00	4330.0
88.00	4141.0
91.00	494.0
92.00	2720.0
93.10	4419.0
94.10	11935.0
95.10	102360.0
96.10	6453.0
97.00	167.0
103.90	496.0
104.90	273.0
105.90	501.0
106.90	166.0
107.90	255.0
111.00	140.0
112.80	128.0
116.00	474.0
117.00	815.0
117.90	476.0
119.00	699.0
128.00	519.0
129.00	163.0
130.00	403.0
131.00	222.0
135.10	176.0
136.90	215.0
139.90	112.0
141.00	1209.0
142.10	173.0
143.00	1730.0
144.00	123.0
145.00	802.0
145.90	168.0
148.00	281.0
149.90	143.0
152.90	133.0
154.90	248.0
157.00	235.0
158.90	130.0
161.00	203.0
172.00	920.0
174.00	82992.0
175.10	6185.0
176.00	80216.0
177.00	4812.0
178.00	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB357