


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV082225\  
Data File : VV039008.D  
Acq On : 22 Aug 2025 07:56  
Operator : SY/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\82V082125W.M  
Title : SW846 8260  
Last Update : Fri Aug 22 04:15:04 2025

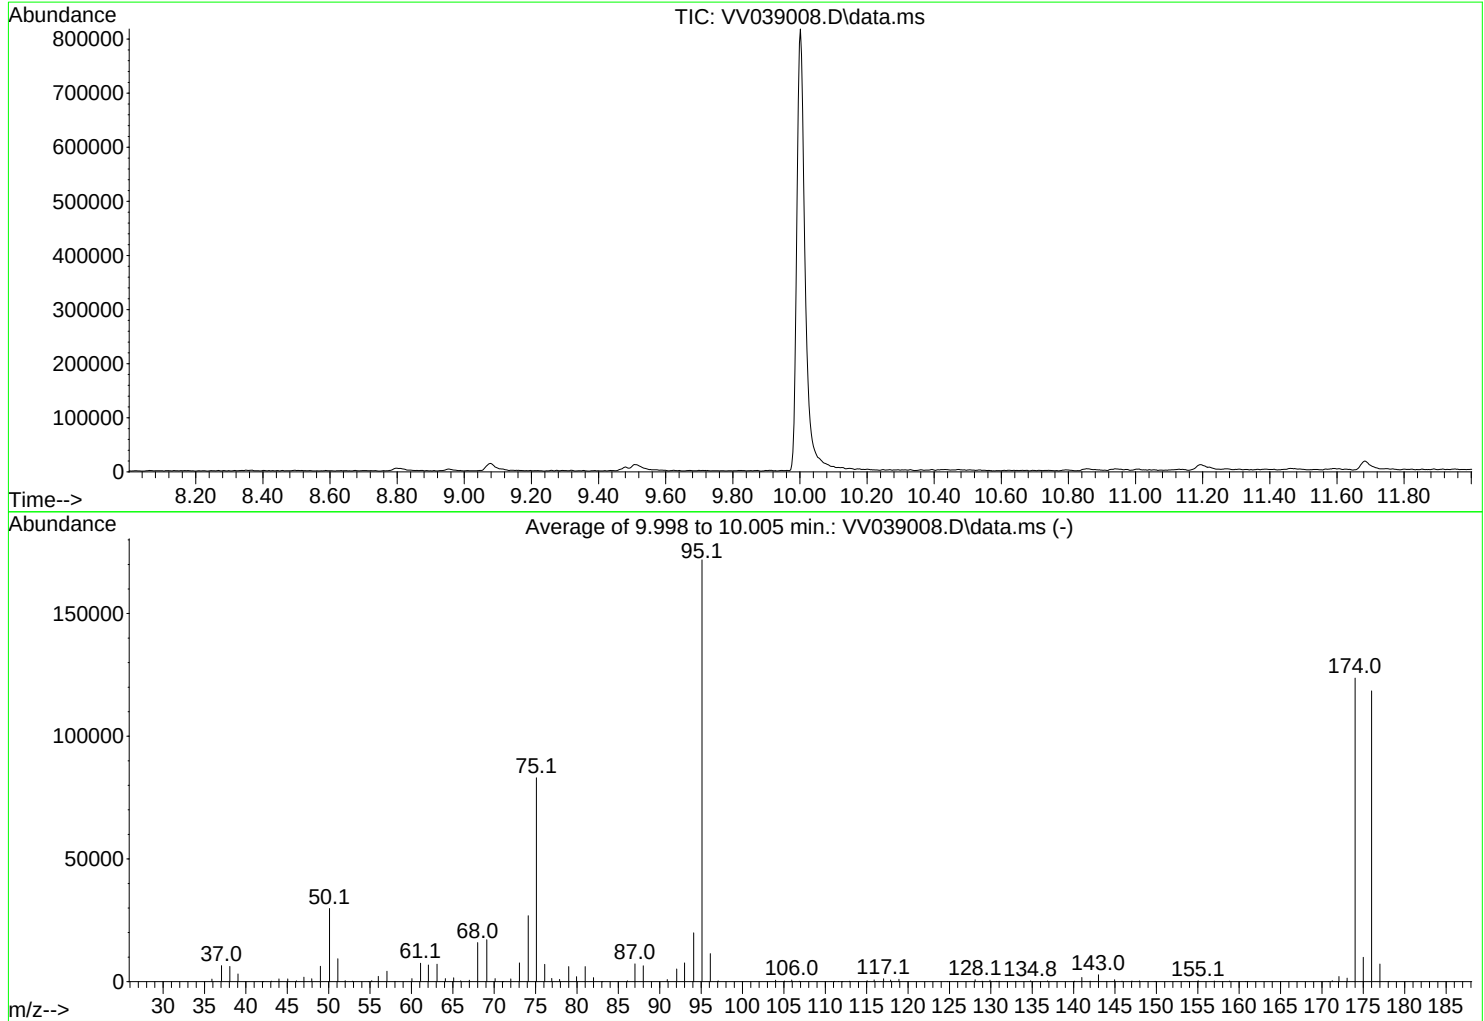

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 17.3  | 29773  | PASS      |
| 75     | 95      | 30     | 60     | 48.3  | 83061  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 171883 | PASS      |
| 96     | 95      | 5      | 9      | 6.6   | 11417  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.1   | 1416   | PASS      |
| 174    | 95      | 50     | 100    | 72.0  | 123715 | PASS      |
| 175    | 174     | 5      | 9      | 8.0   | 9904   | PASS      |
| 176    | 174     | 95     | 101    | 95.8  | 118488 | PASS      |
| 177    | 176     | 5      | 9      | 6.1   | 7173   | PASS      |