

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082318\
 Data File : VV007156.D
 Acq On : 23 Aug 2018 22:13
 Operator : SY/MD
 Sample : J4622-13
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK5

Manual Integrations
 APPROVED

sam
 8/24/2018 3:00:38 PM

Quant Time: Aug 24 02:53:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 24 02:07:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	539158	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	512482	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	188346	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	141214	41.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.36%
7) Chloroethane-d5	1.57	69	124575m	57.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	114.34%
11) 1,1-Dichloroethene-d2	2.13	63	206406	32.90	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.80%
21) 2-Butanone-d5	3.95	46	282392	97.92	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.92%
24) Chloroform-d	4.41	84	345052	47.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.09	65	218420	49.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.40%
32) Benzene-d6	5.10	84	669209	46.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.96%
36) 1,2-Dichloropropane-d6	6.12	67	232558	49.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.72%
41) Toluene-d8	7.37	98	518465	41.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.74%
43) trans-1,3-Dichloropropene-	7.67	79	86334	42.80	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.60%
47) 2-Hexanone-d5	8.14	63	117751	70.28	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	70.28%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	308681	45.03	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.06%
64) 1,2-Dichlorobenzene-d4	11.68	152	189774	50.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.22%

Target Compounds

					Ovalue
5) Vinyl chloride	1.32	62	7235	1.41 ug/L	# 74
20) cis-1,2-Dichloroethene	3.96	96	20827	4.60 ug/L	90
34) Trichloroethene	5.96	95	16823	4.04 ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082318\
Data File : VV007156.D
Acq On : 23 Aug 2018 22:13
Operator : SY/MD
Sample : J4622-13
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
ETBK5

Manual Integrations
APPROVED

sam
8/24/2018 3:00:38 PM

Quant Time: Aug 24 02:53:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM082218WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 24 02:07:07 2018
Response via : Initial Calibration

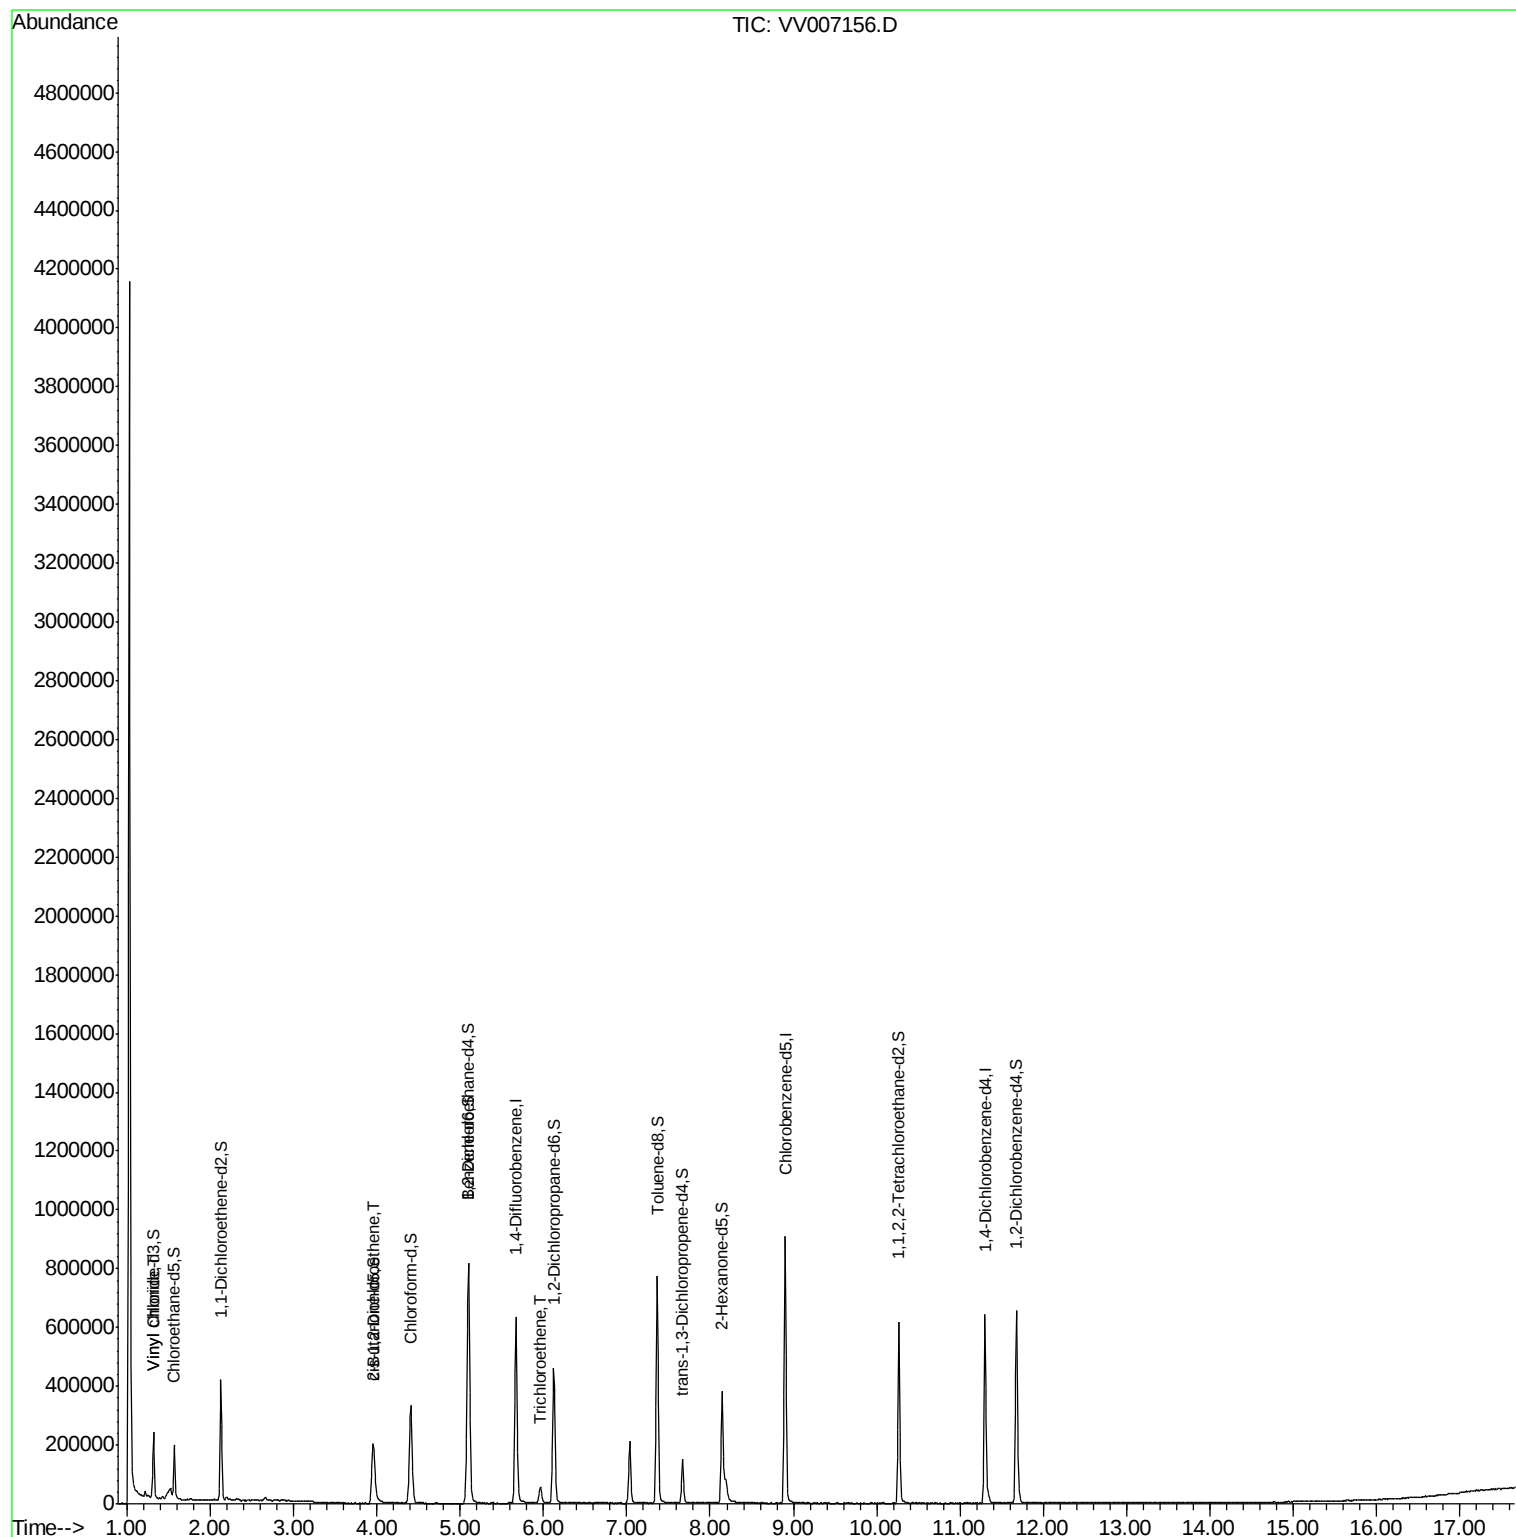

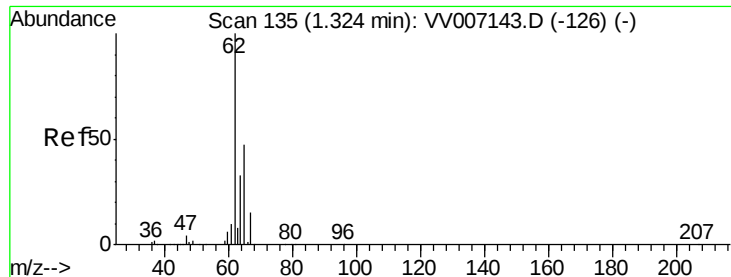

#5

Vinyl chloride

Concen: 1.41 ug/L

RT: 1.32 min Scan# 135

Delta R.T. 0.00 min

Lab File: VV007156.D





Acq: 23 Aug 2018 22:13

Instrument :
MSVOA_V
ClientSampleId :
ETBK5

Tot Ion	Ratio	Lower	Upper
62	100		
64	48.0	23.4	43.4#

Manual Integrations
APPROVED

sam
8/24/2018 3:00:38 PM

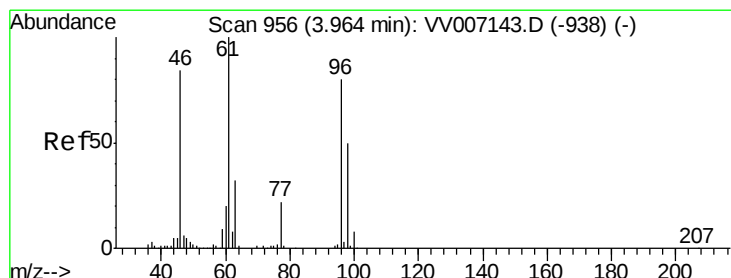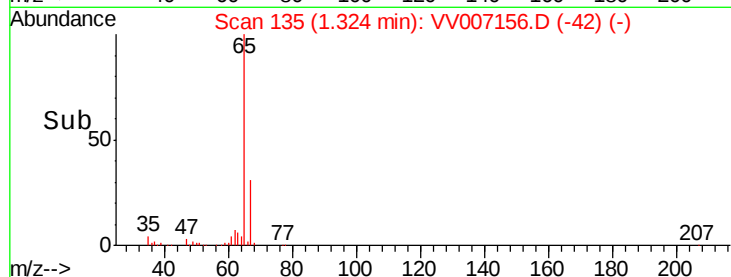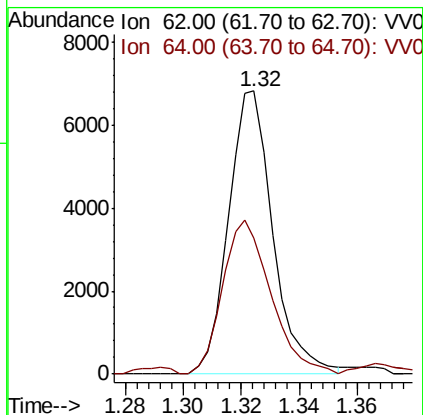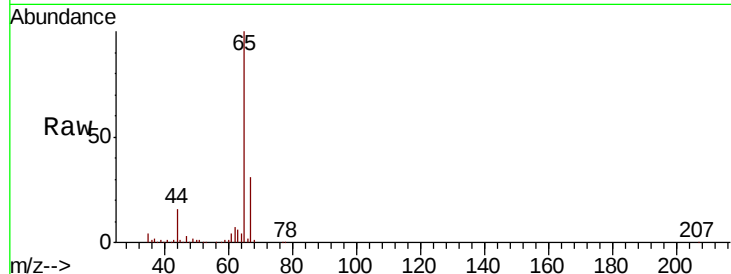

#20

cis-1,2-Dichloroethene

Concen: 4.60 ug/L




RT: 3.96 min Scan# 956


Delta R.T. 0.00 min

Lab File: VV007156.D

Acq: 23 Aug 2018 22:13

Tgt Ion	Ratio	Lower	Upper
96	100		
61	116.2	89.0	165.4
68	0.0	0.0	0.0

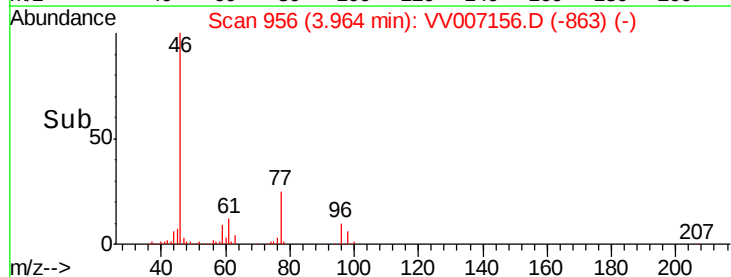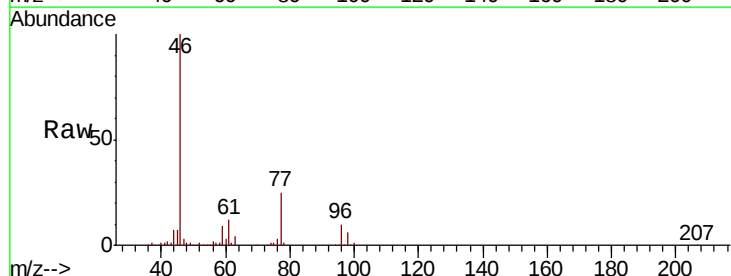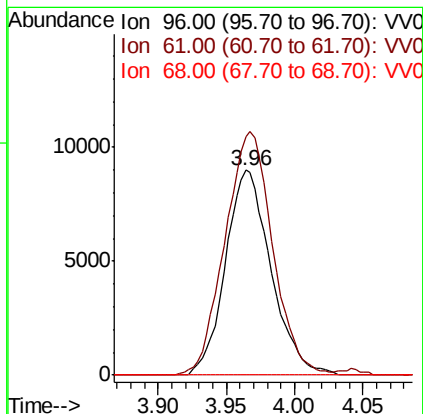

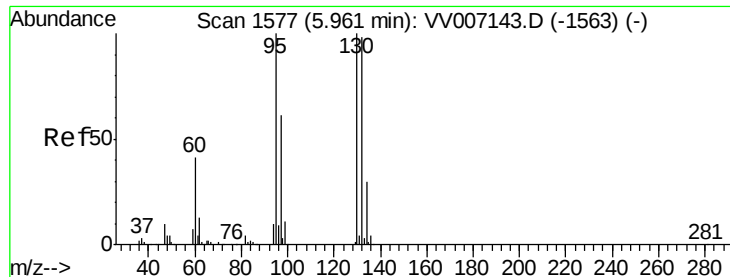

#34
 Trichloroethene
 Concen: 4.04 ug/L
 RT: 5.96 min Scan# 1578
 Delta R.T. 0.00 min
 Lab File: VV007156.D
 Acq: 23 Aug 2018 22:13

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBK5

Tot Ion:	95	Resp:	16823
Ion Ratio	Lower	Upper	
95	100		
97	59.6	45.1	83.9
132	91.7	69.7	129.4
130	98.4	73.6	136.6

Manual Integrations
 APPROVED

sam
 8/24/2018 3:00:38 PM

